

1 μ m

Mag = 12.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_01.tif



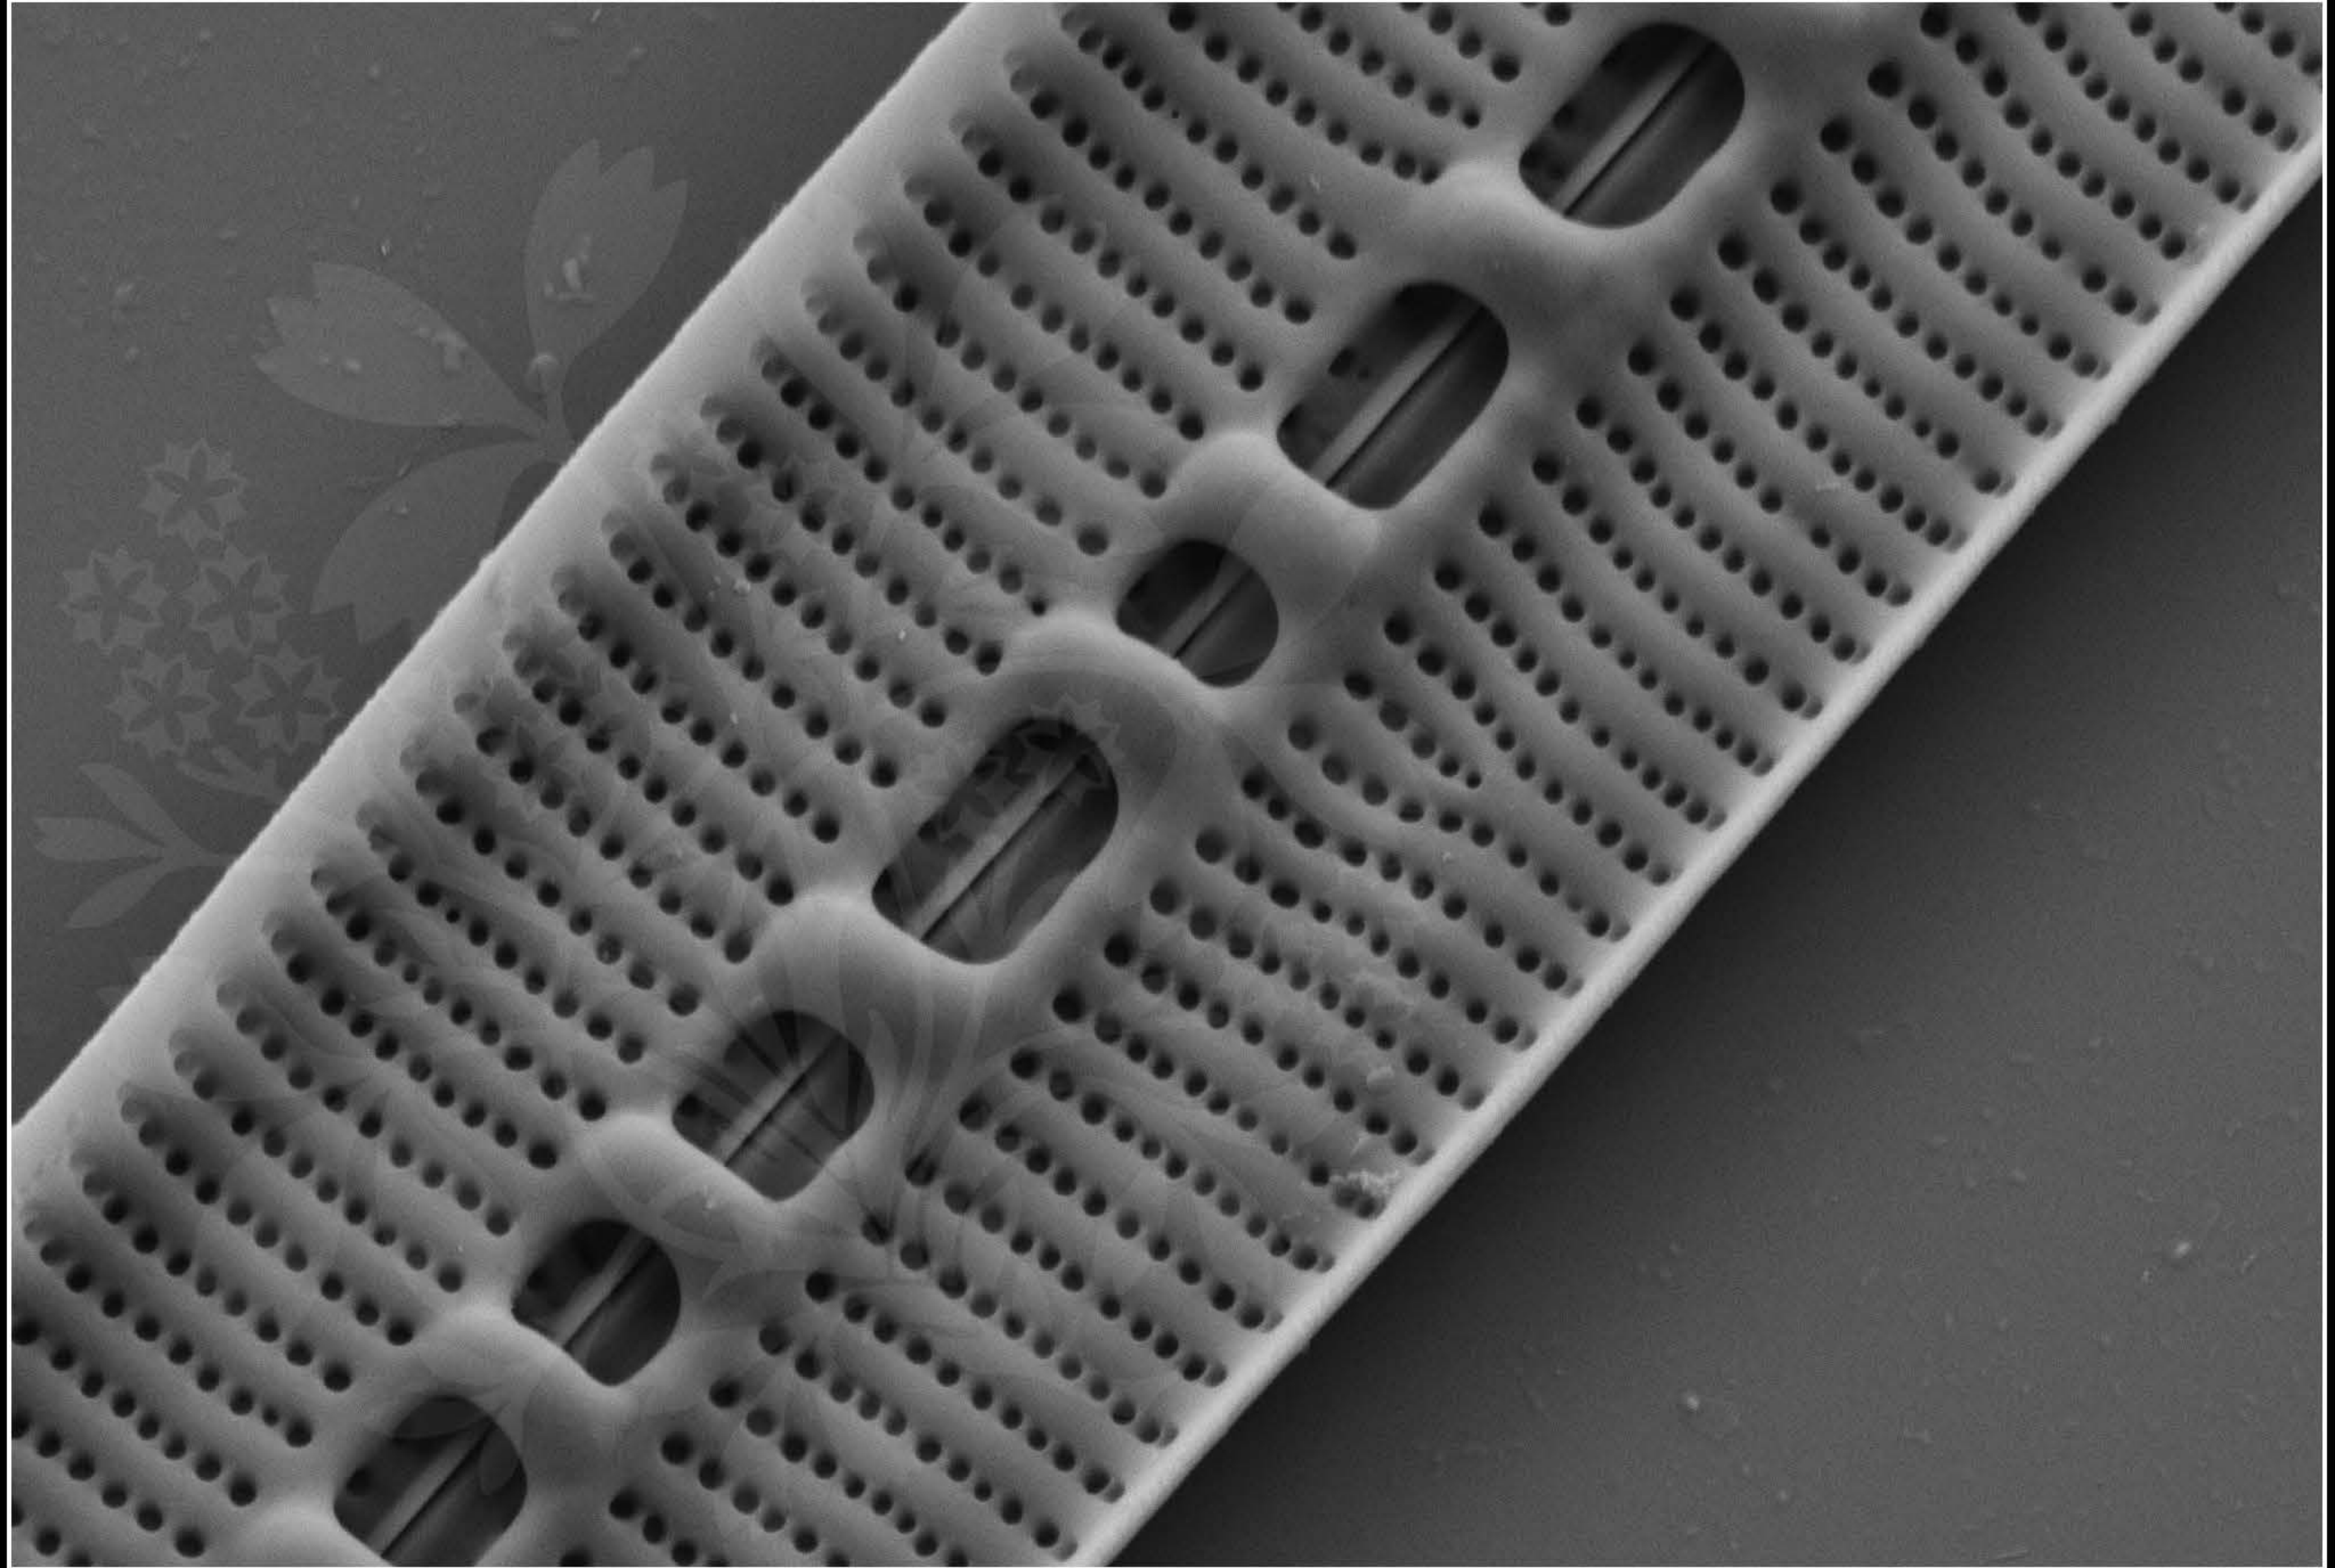

1 μm

Mag = 20.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_02.tif



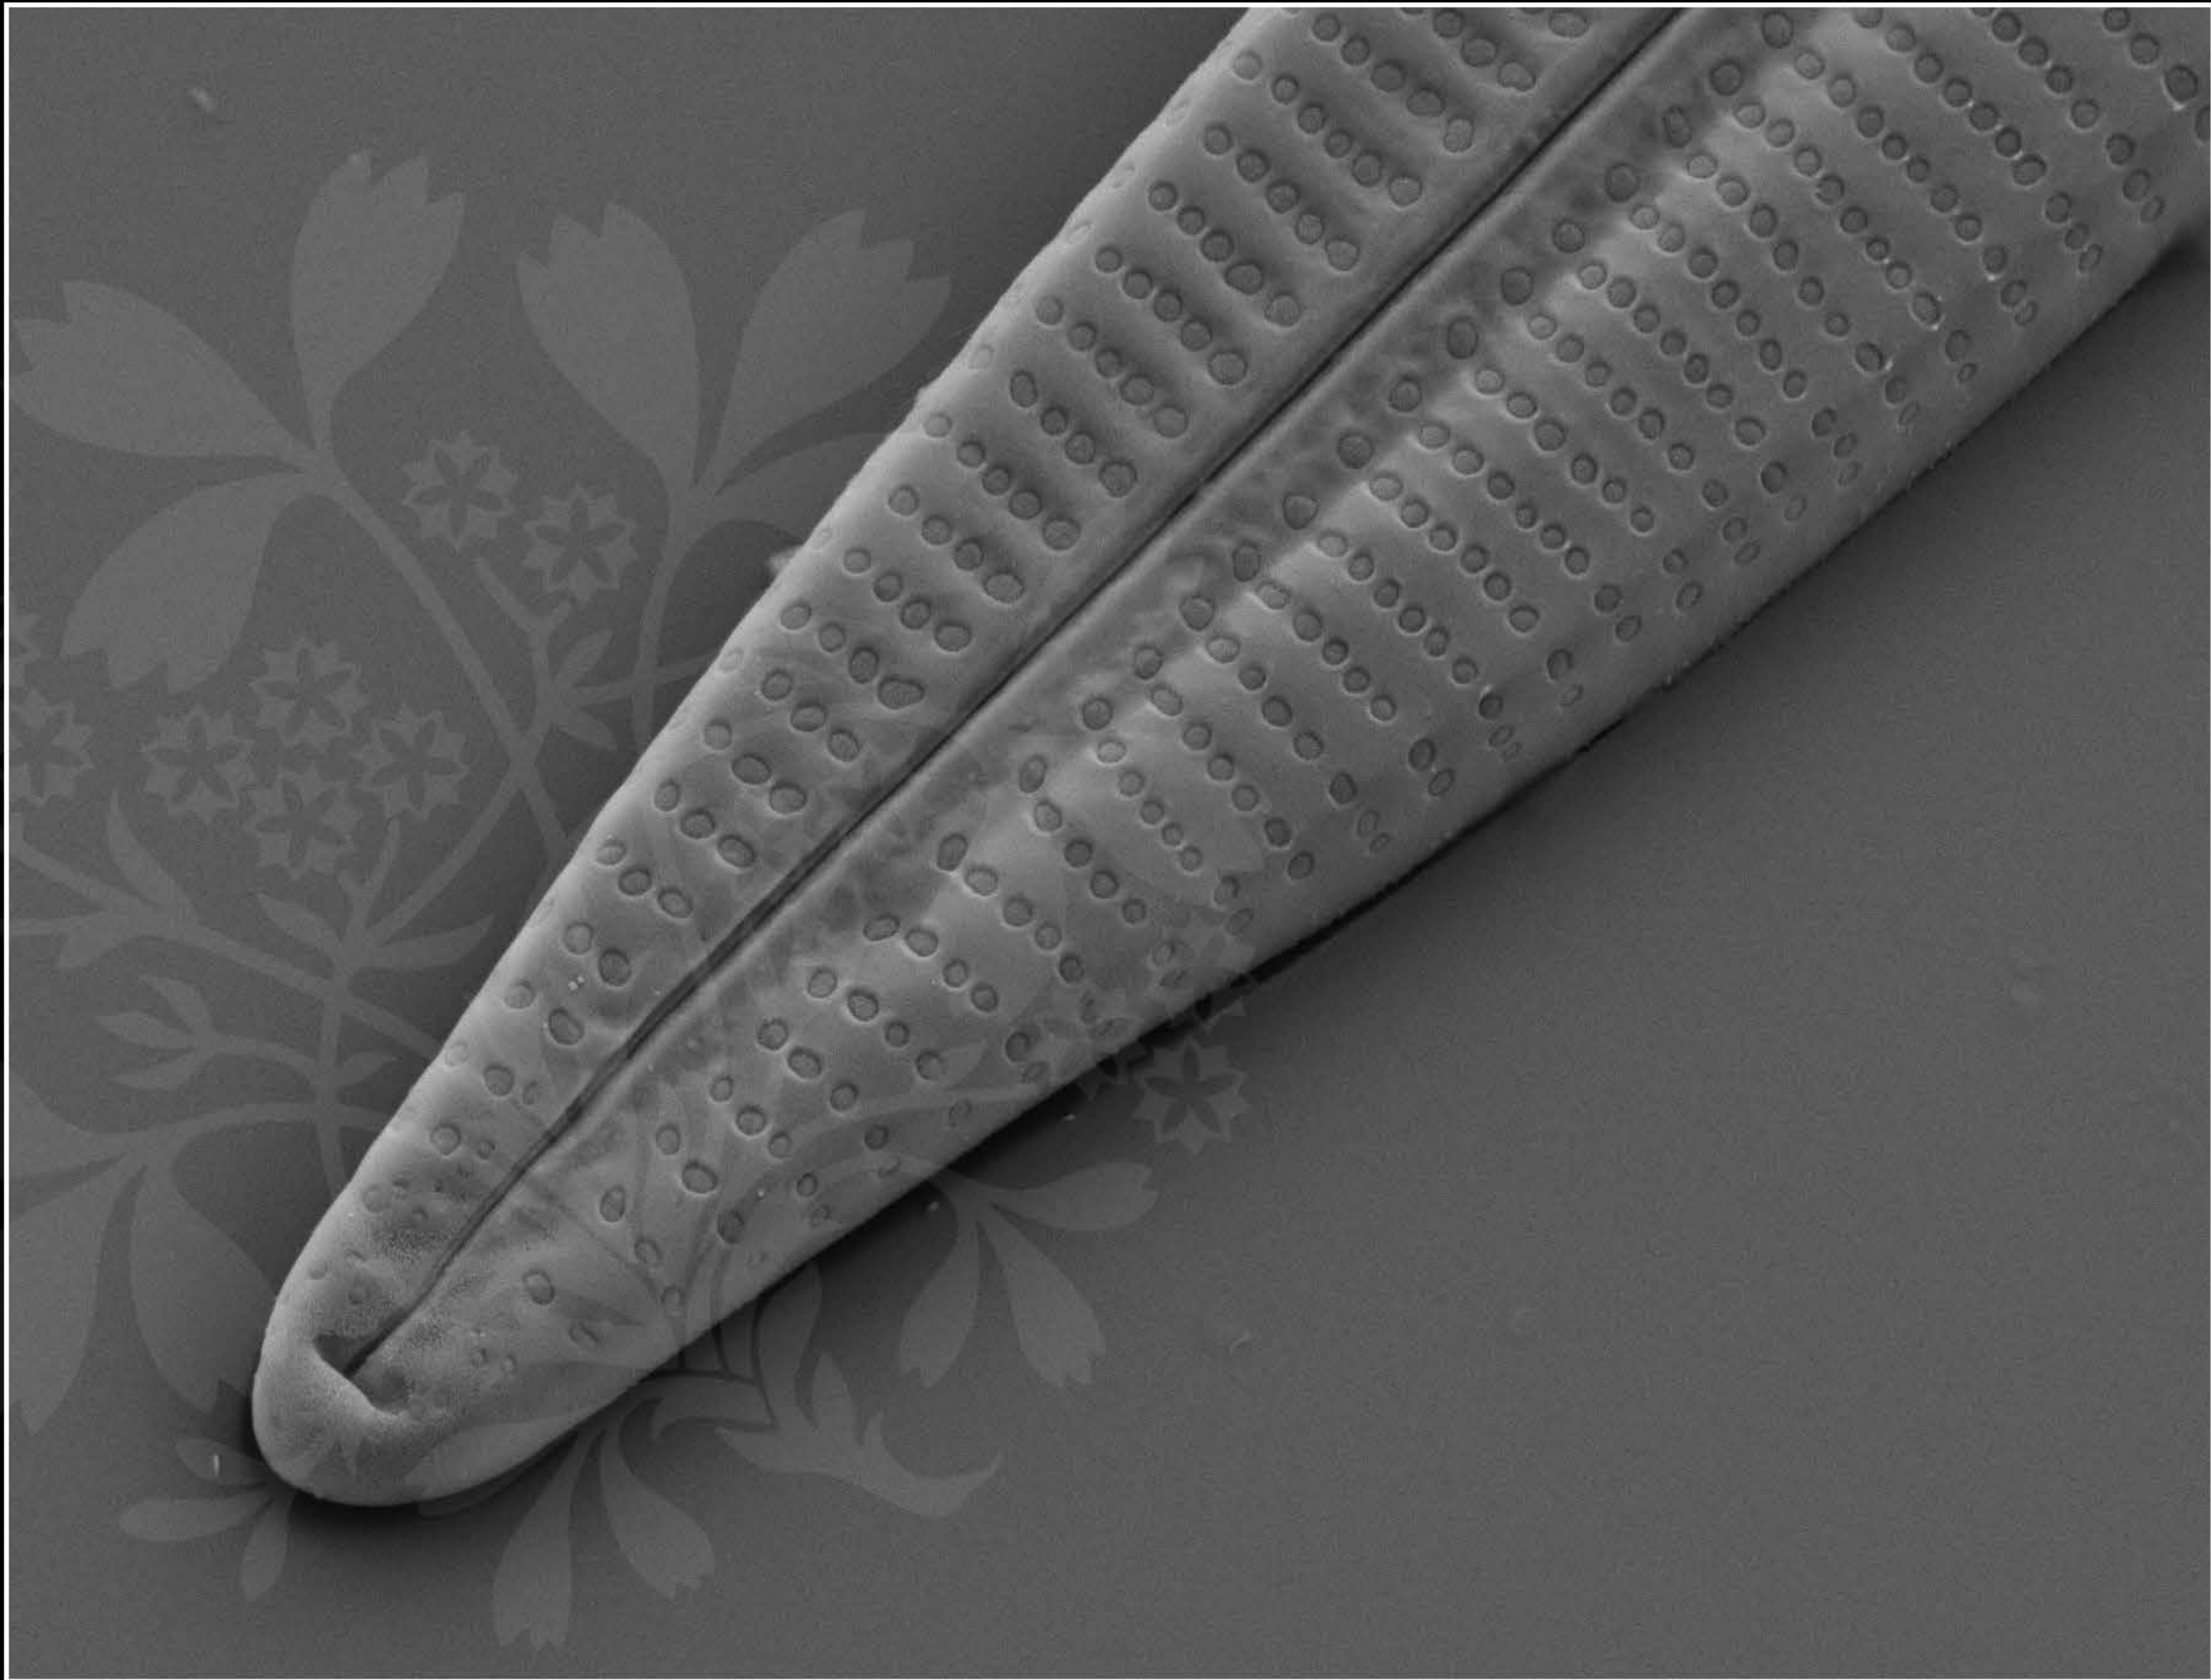

1 μm

Mag = 20.00 K X

EHT = 4.50 kV


Signal A = SE2

Date : 3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_03.tif



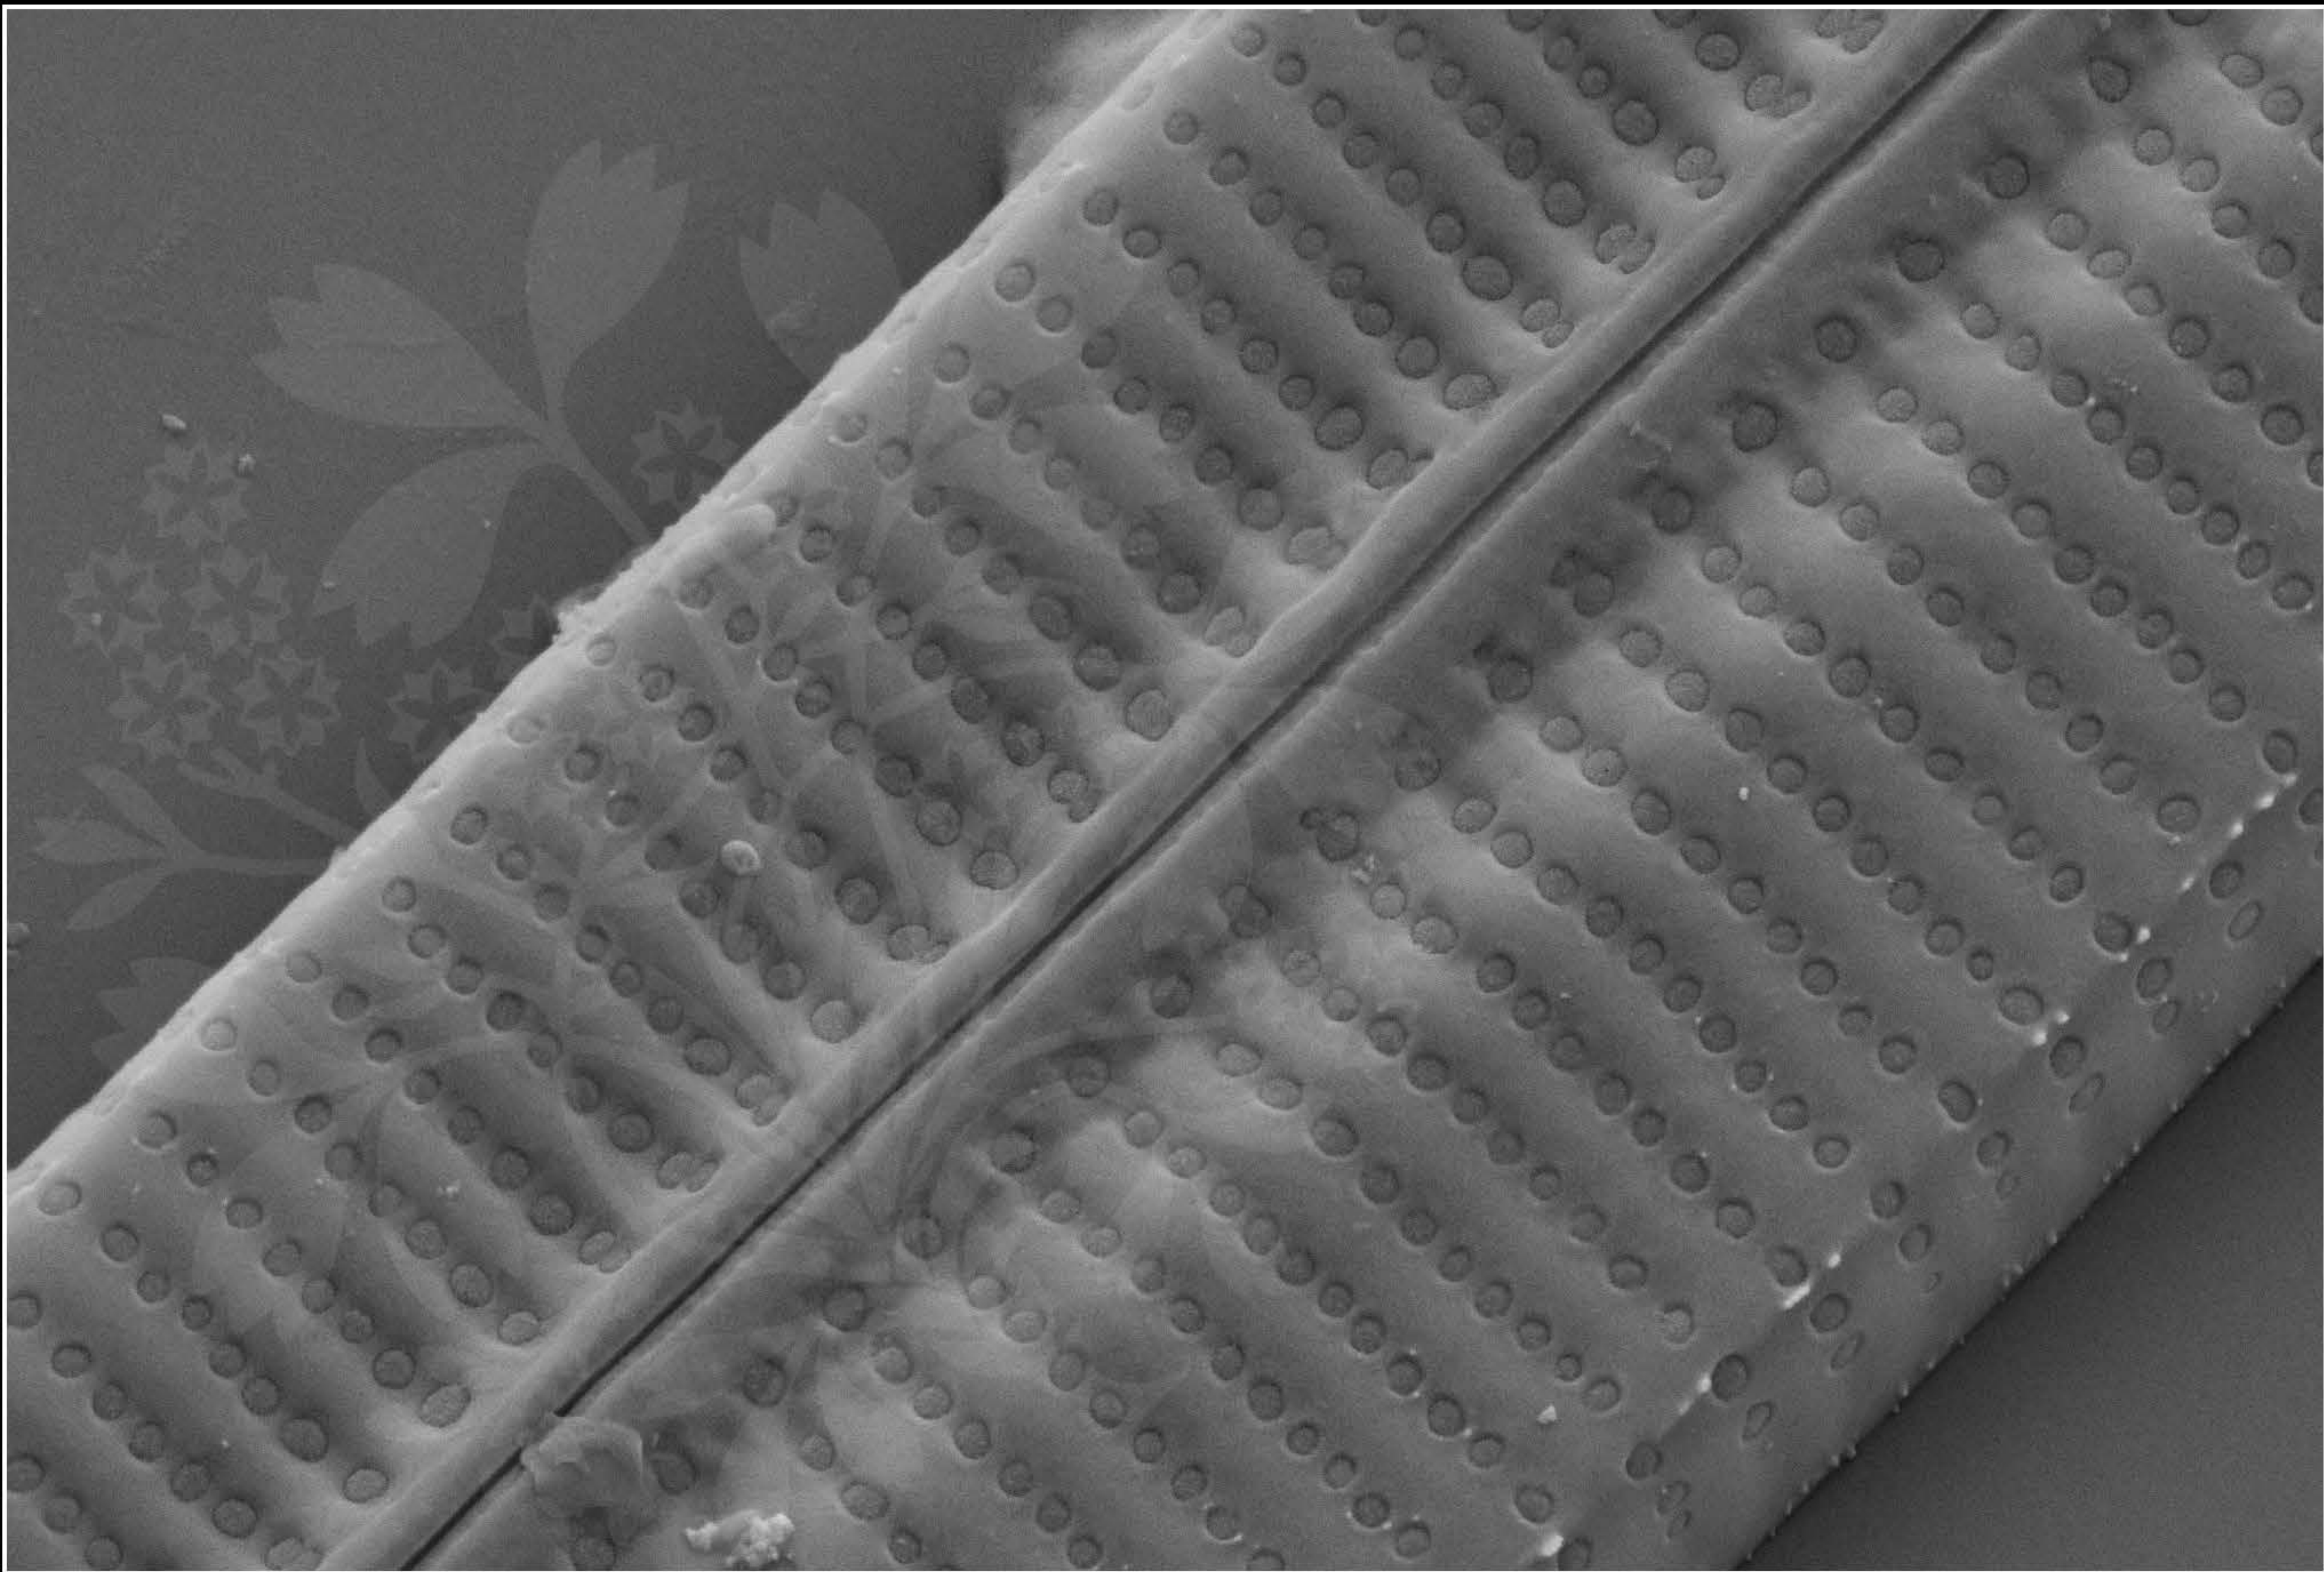

200 nm
└─┘

Mag = 30.00 K X

EHT = 4.50 kV


Signal A = SE2

Date : 3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_04.tif



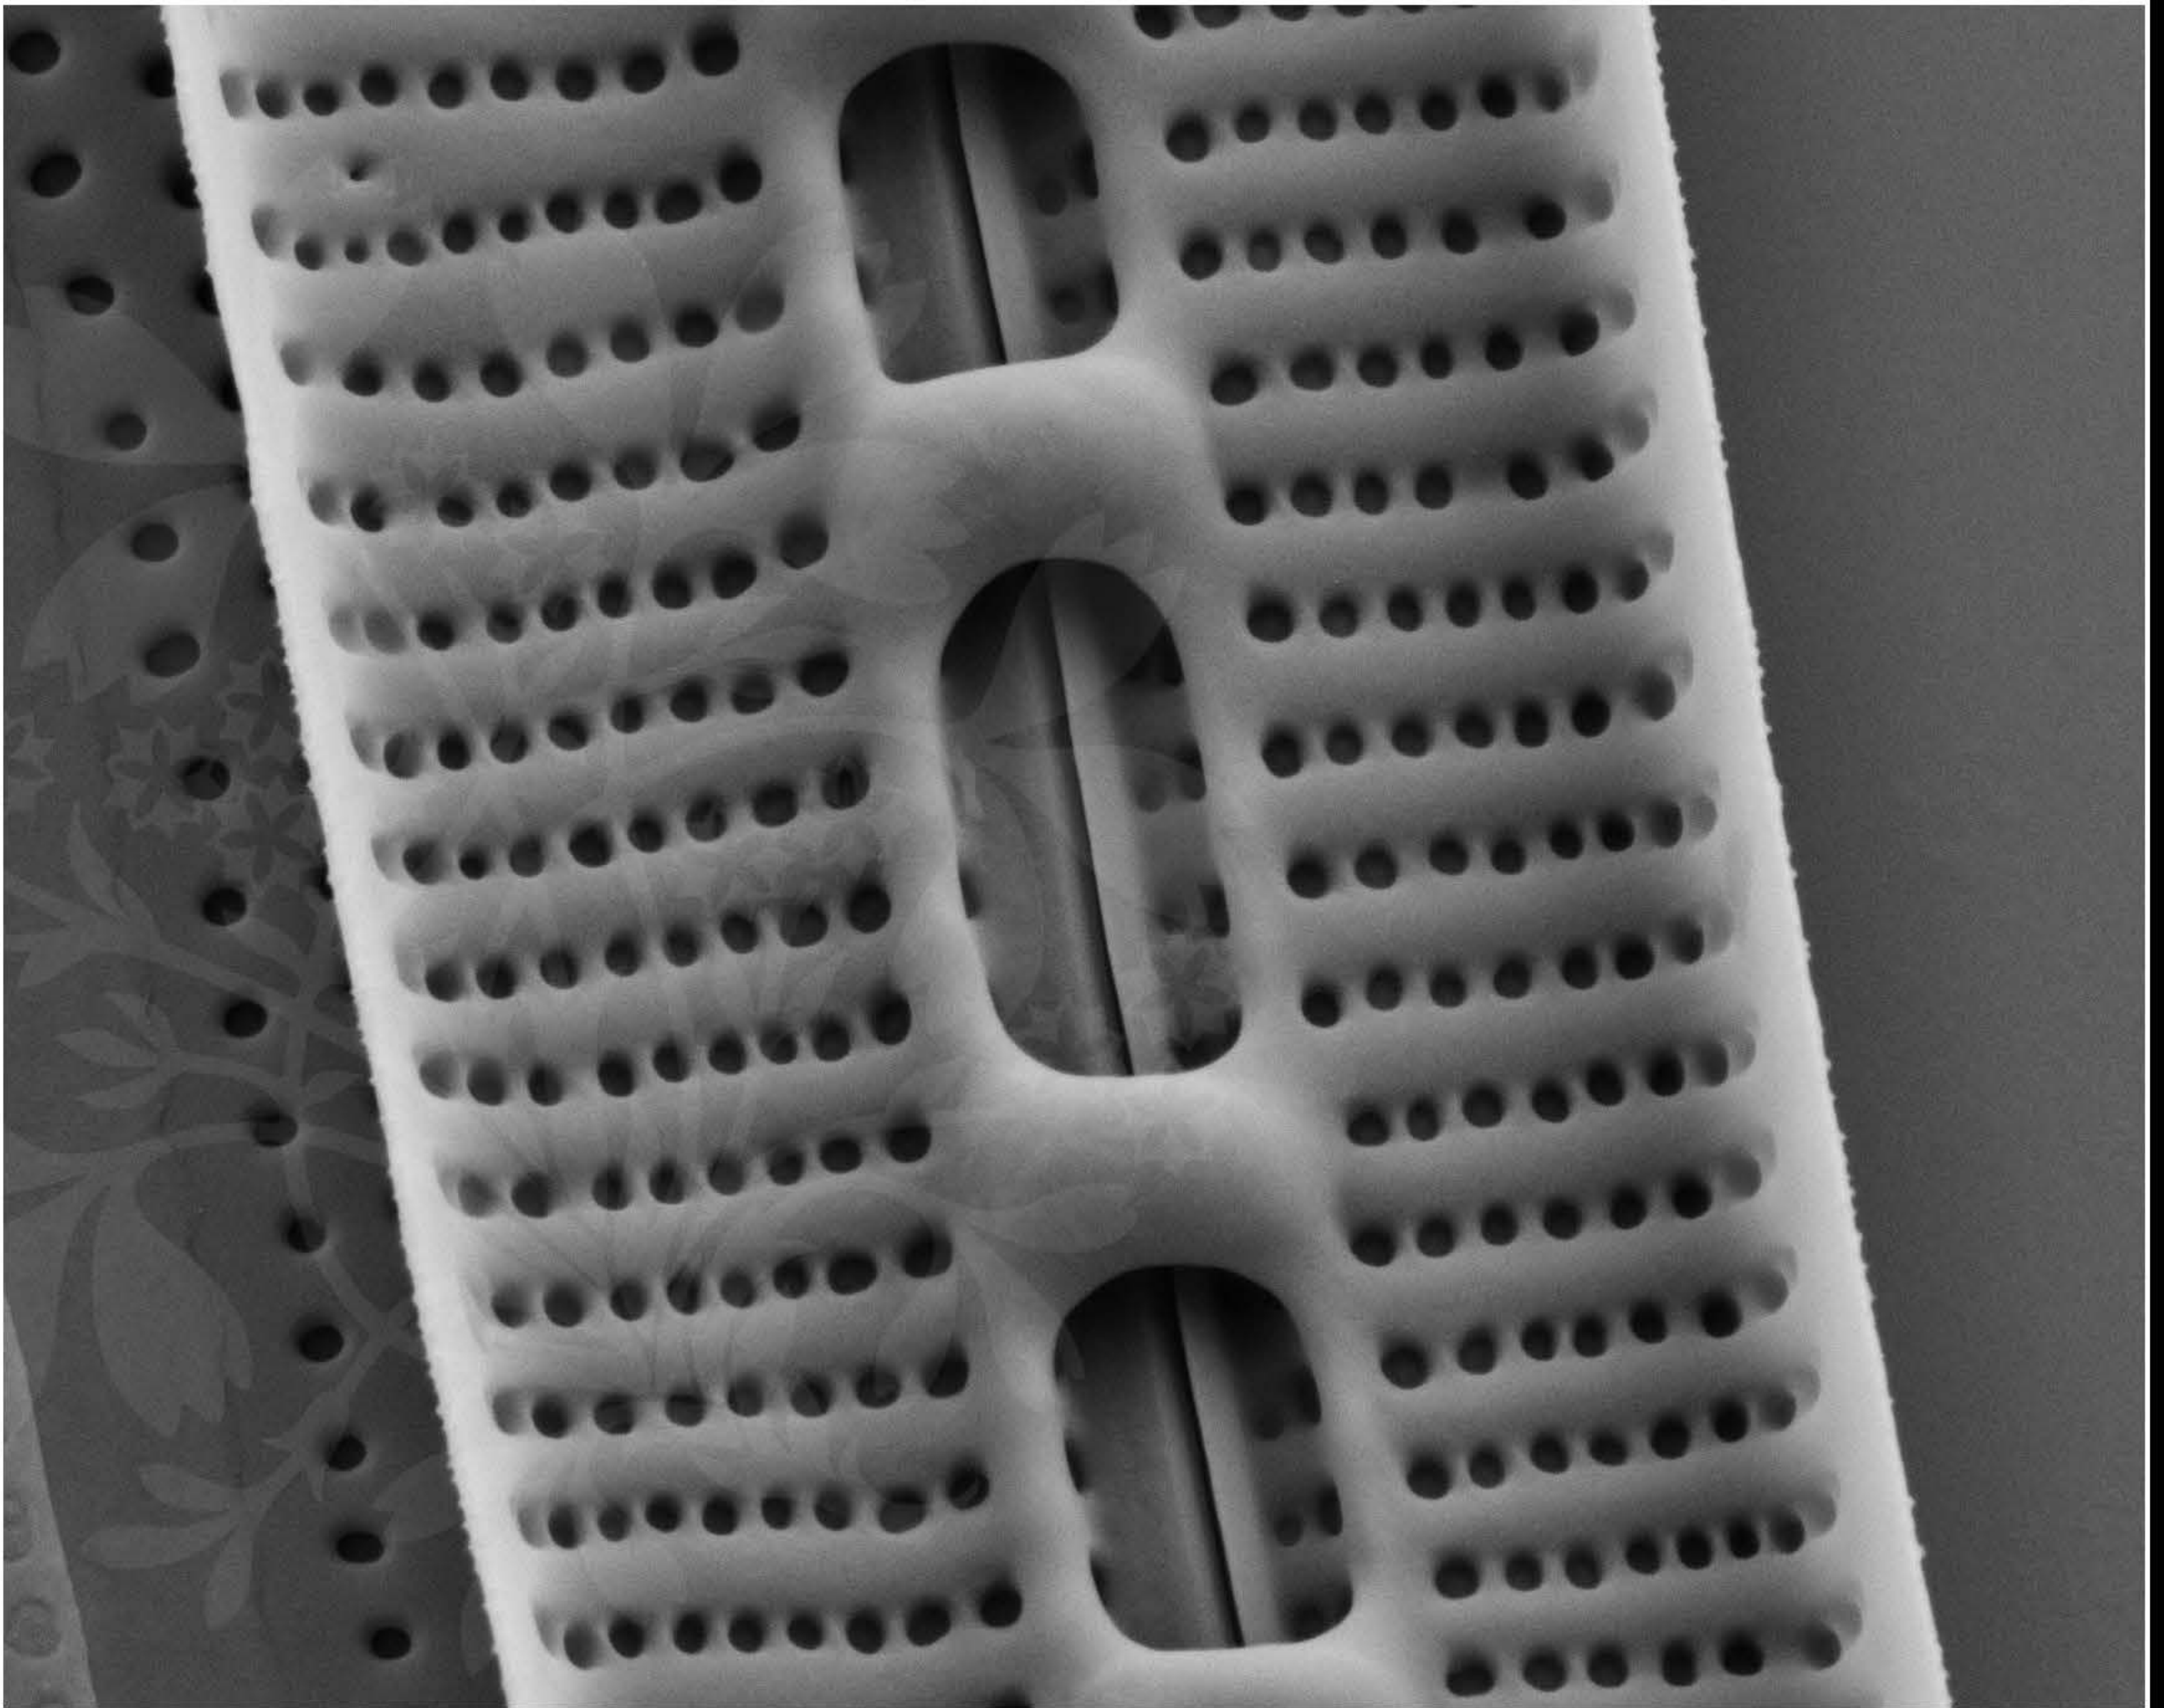

200 nm
└─┘

Mag = 30.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_05.tif



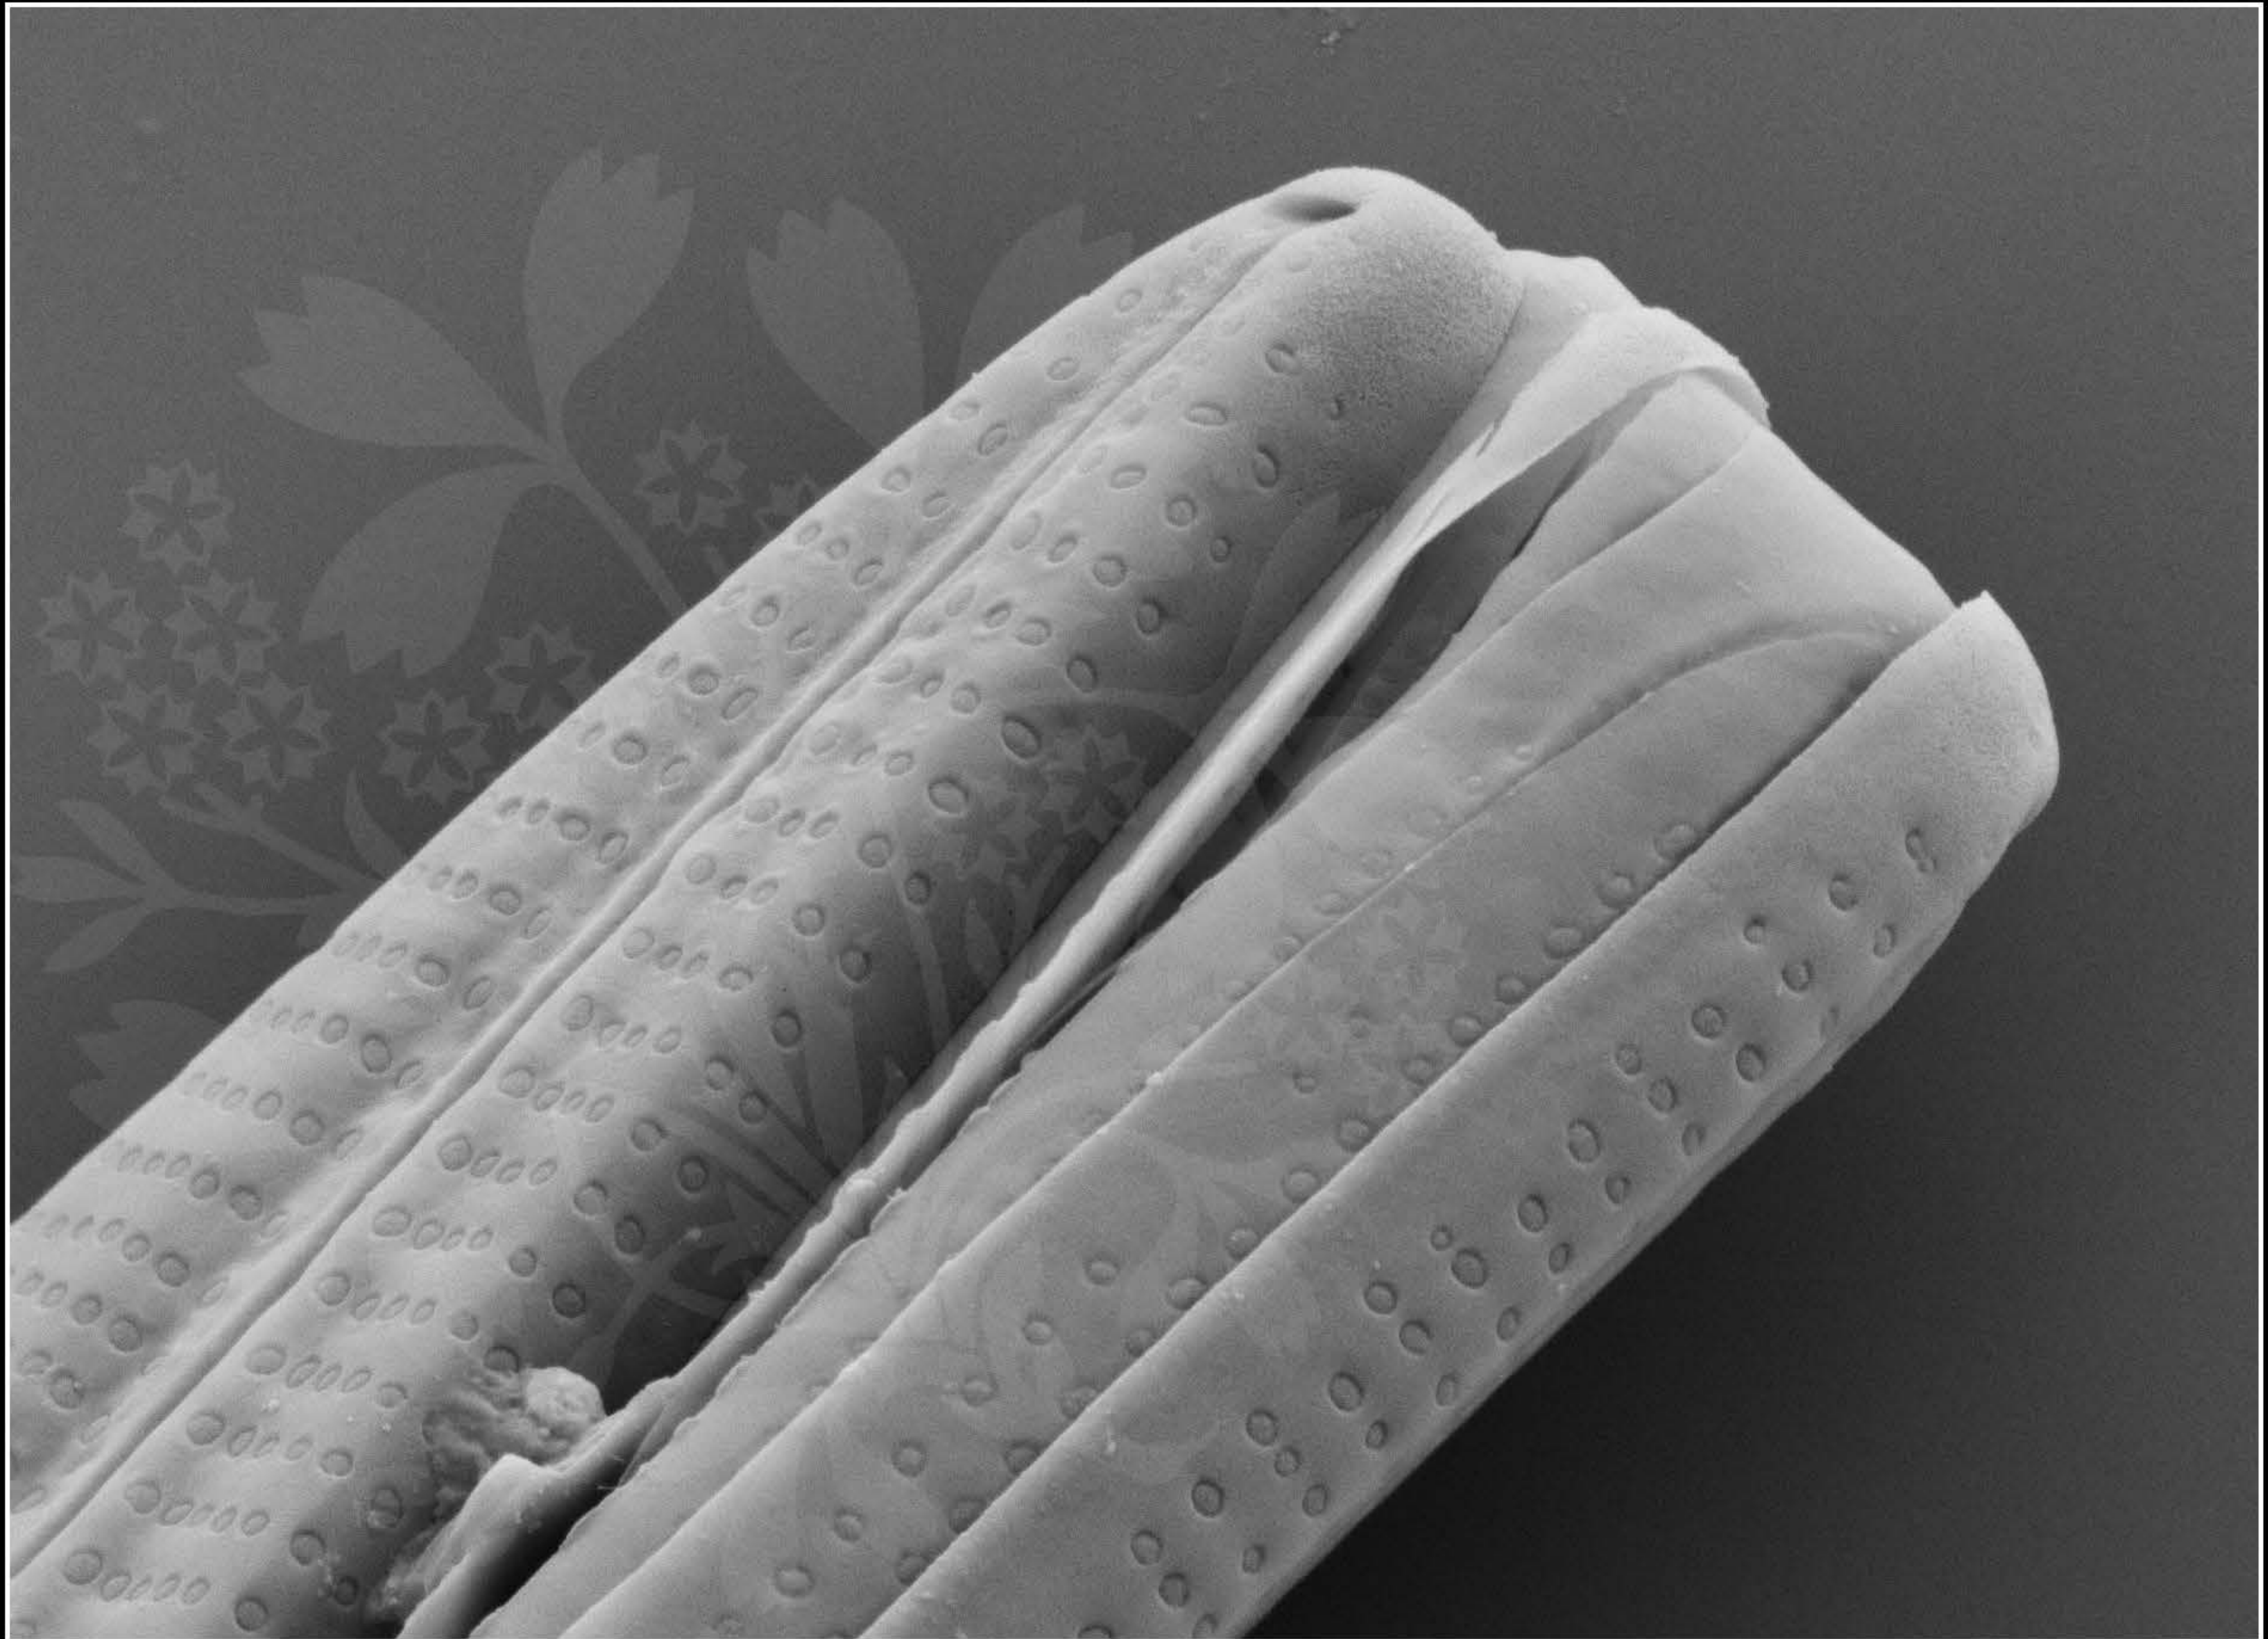

300 nm
└───┘

Mag = 25.00 K X


EHT = 4.50 kV

Signal A = SE2 Date : 3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_06.tif



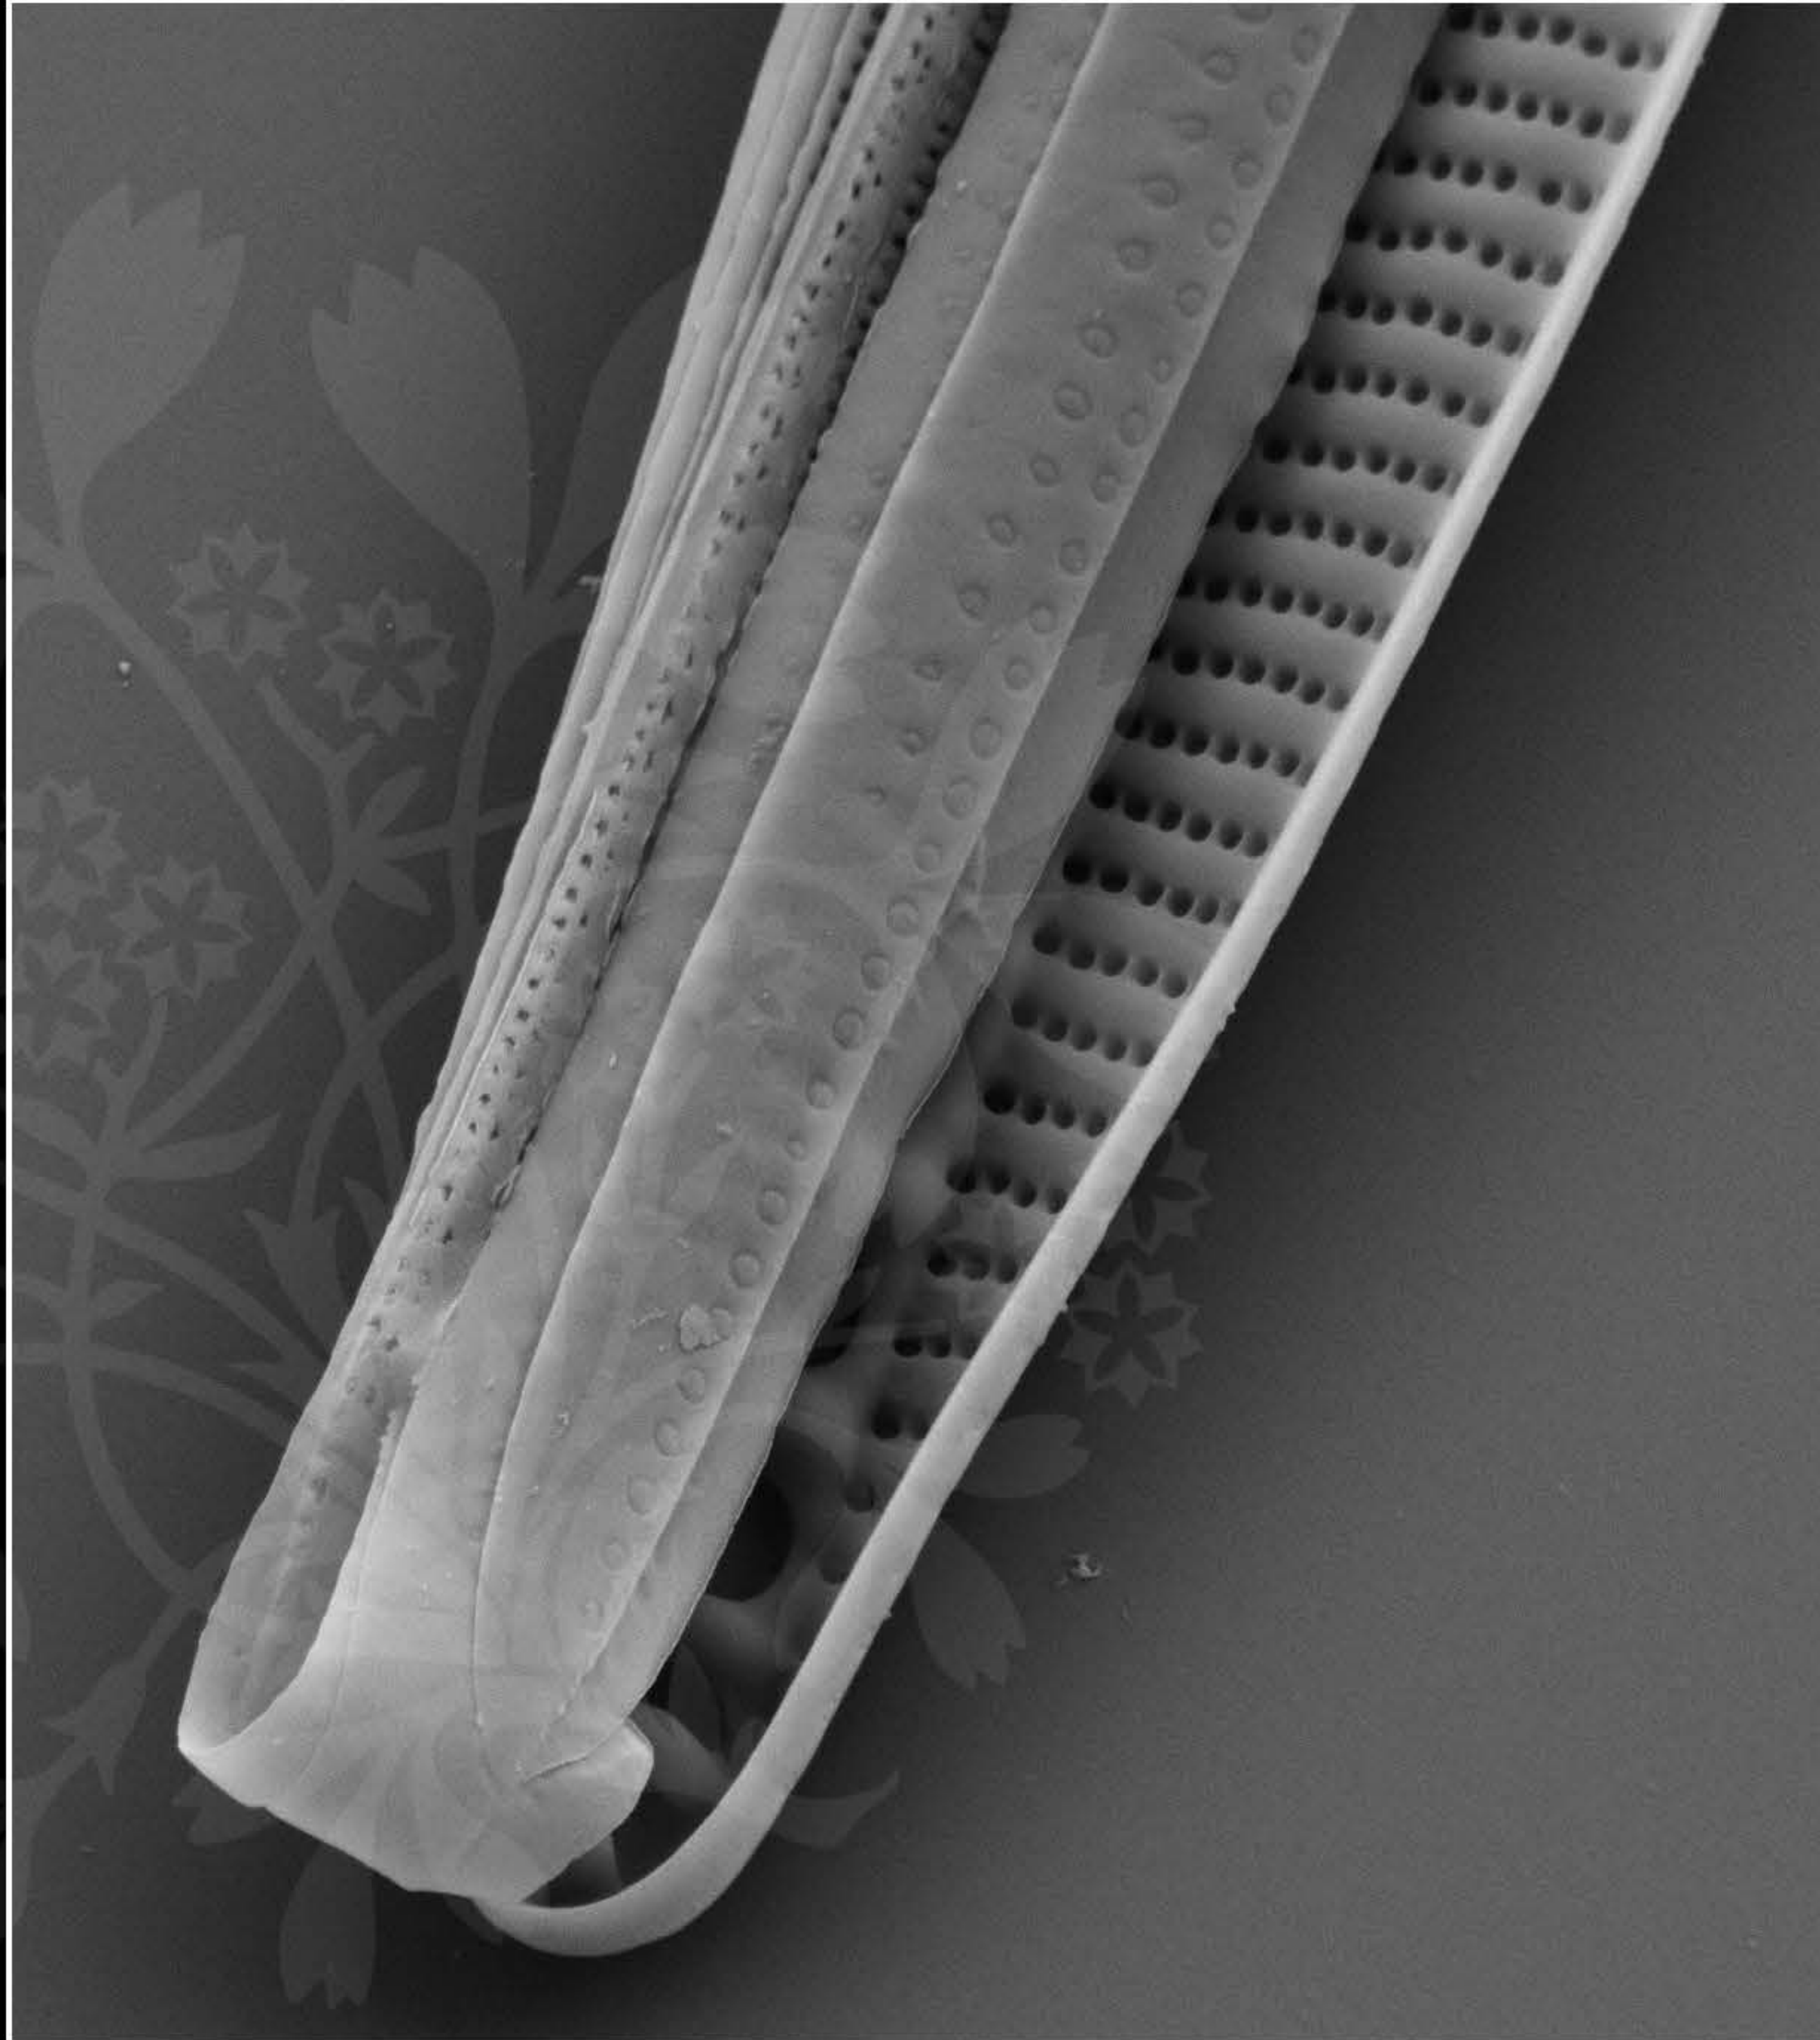

1 μm

Mag = 16.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_07.tif



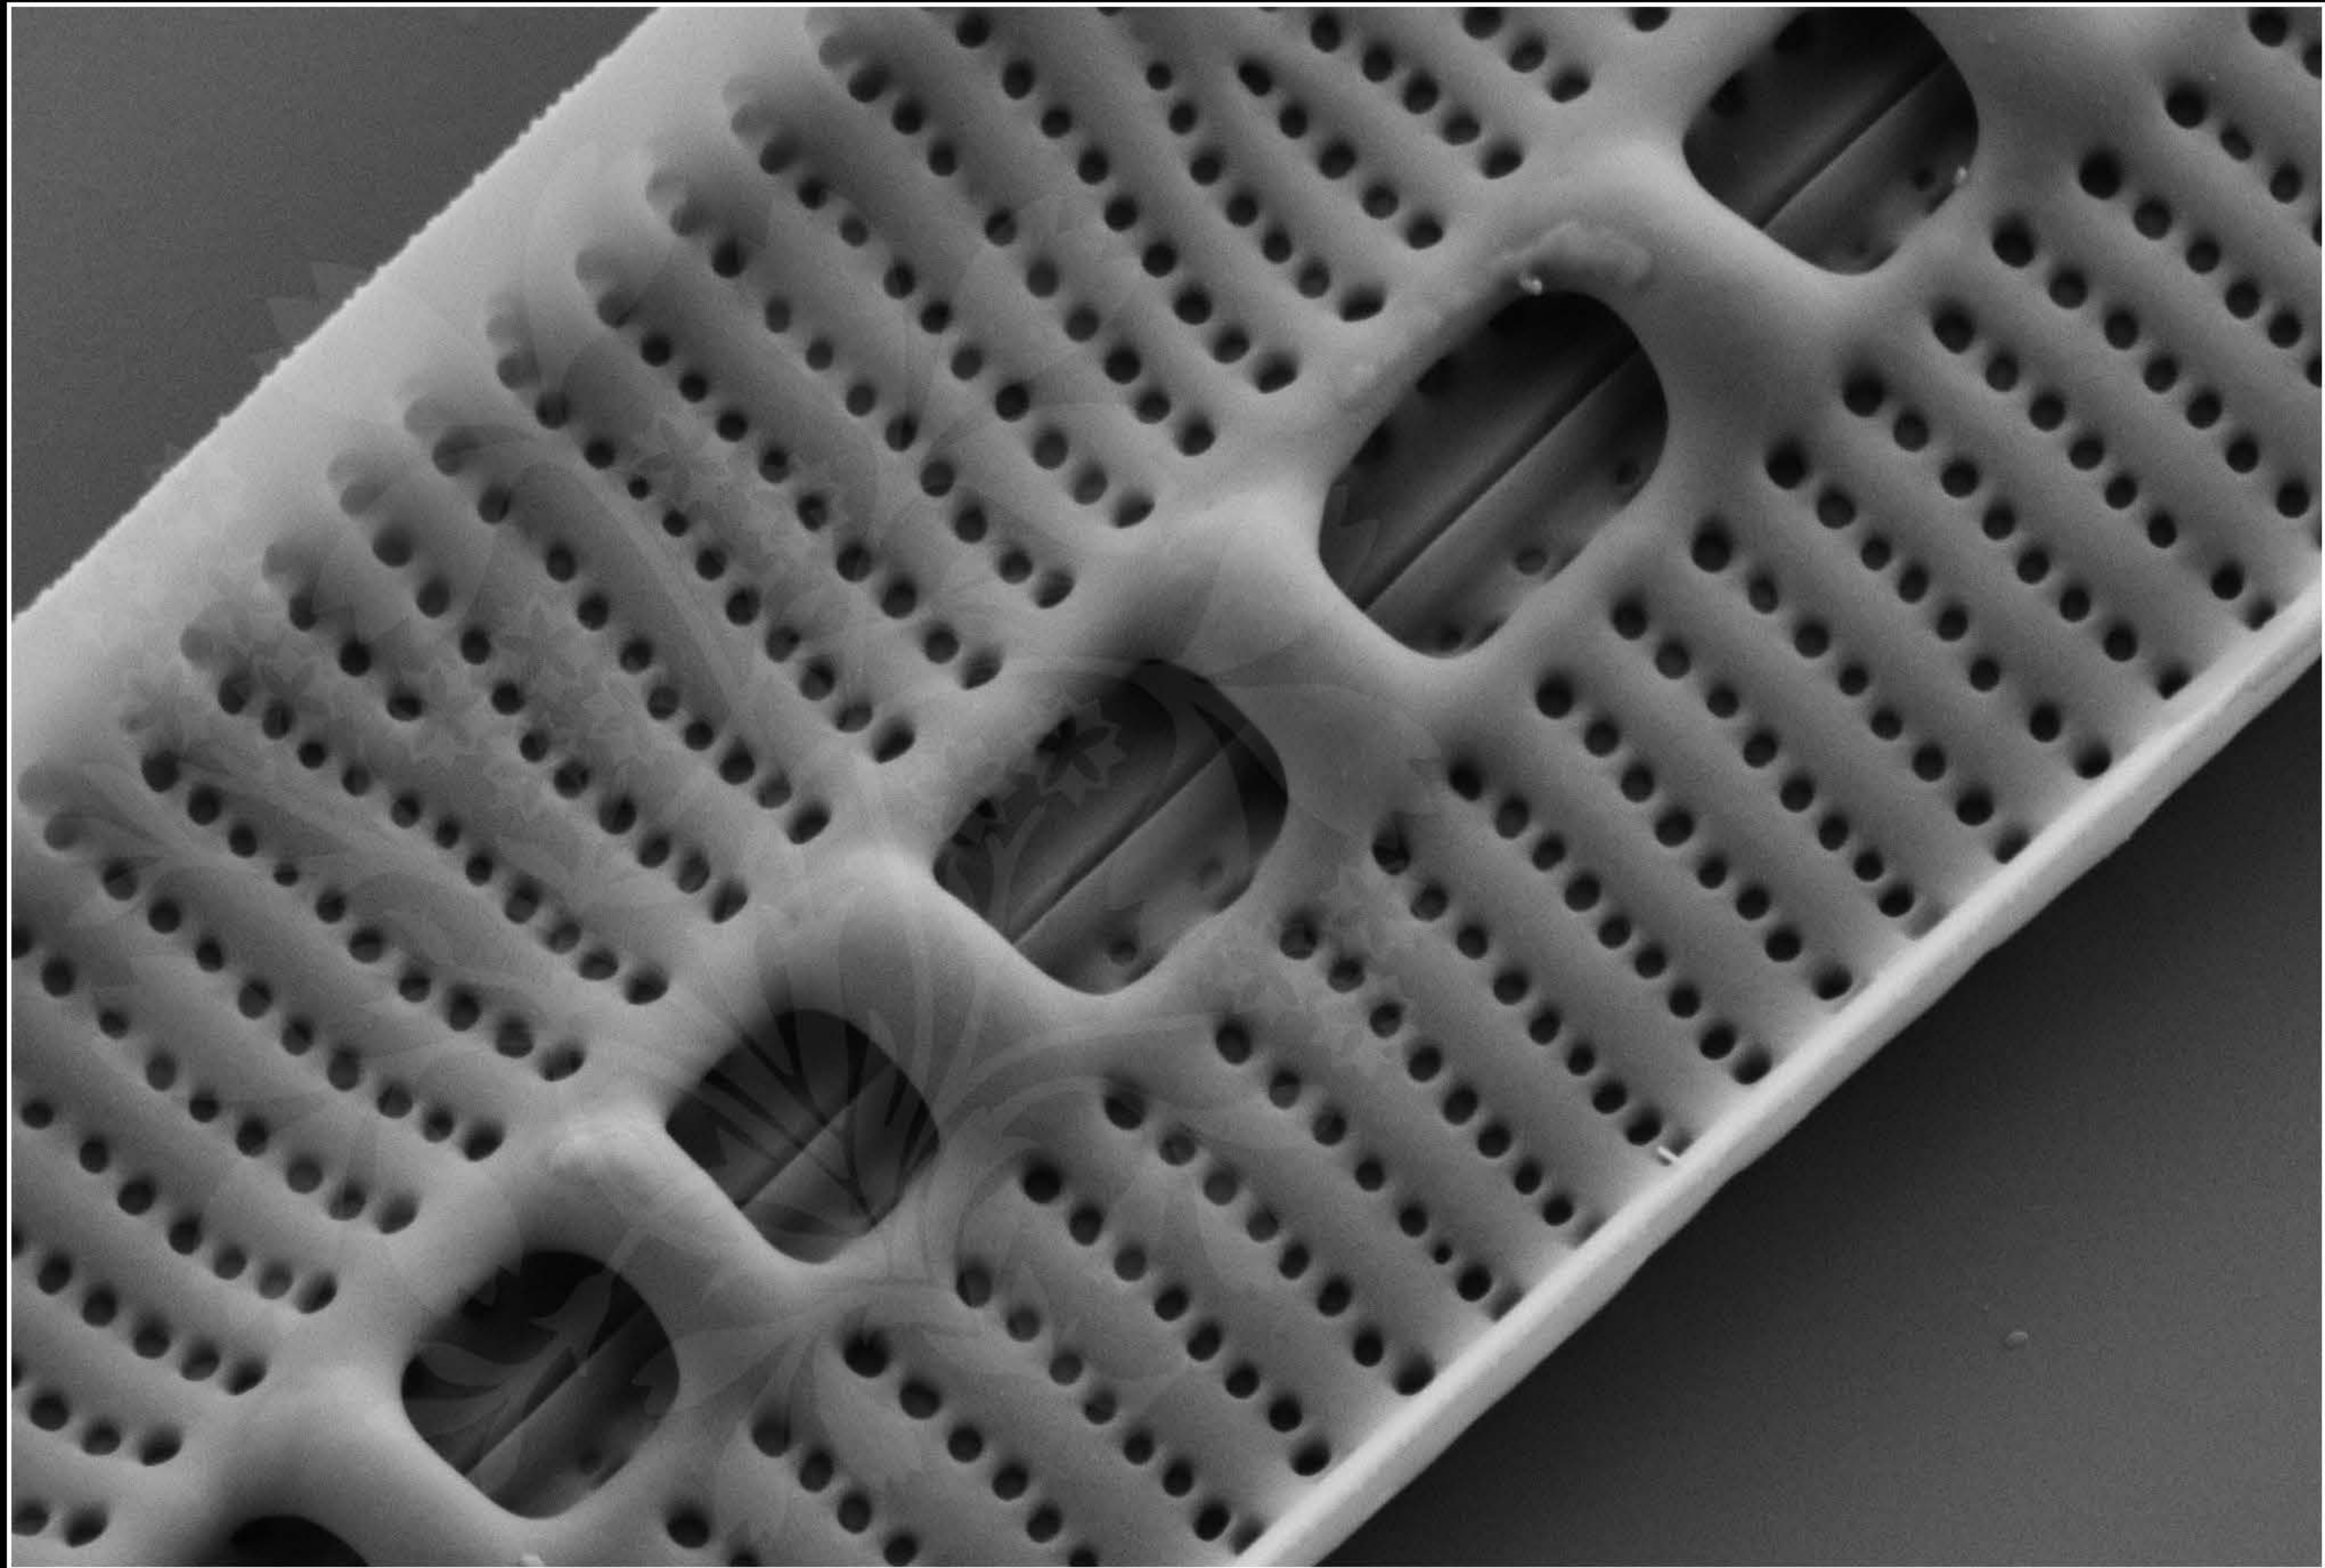

200 nm
└─┘

Mag = 30.00 K X


EHT = 4.50 kV

Signal A = SE2 Date : 3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_08.tif



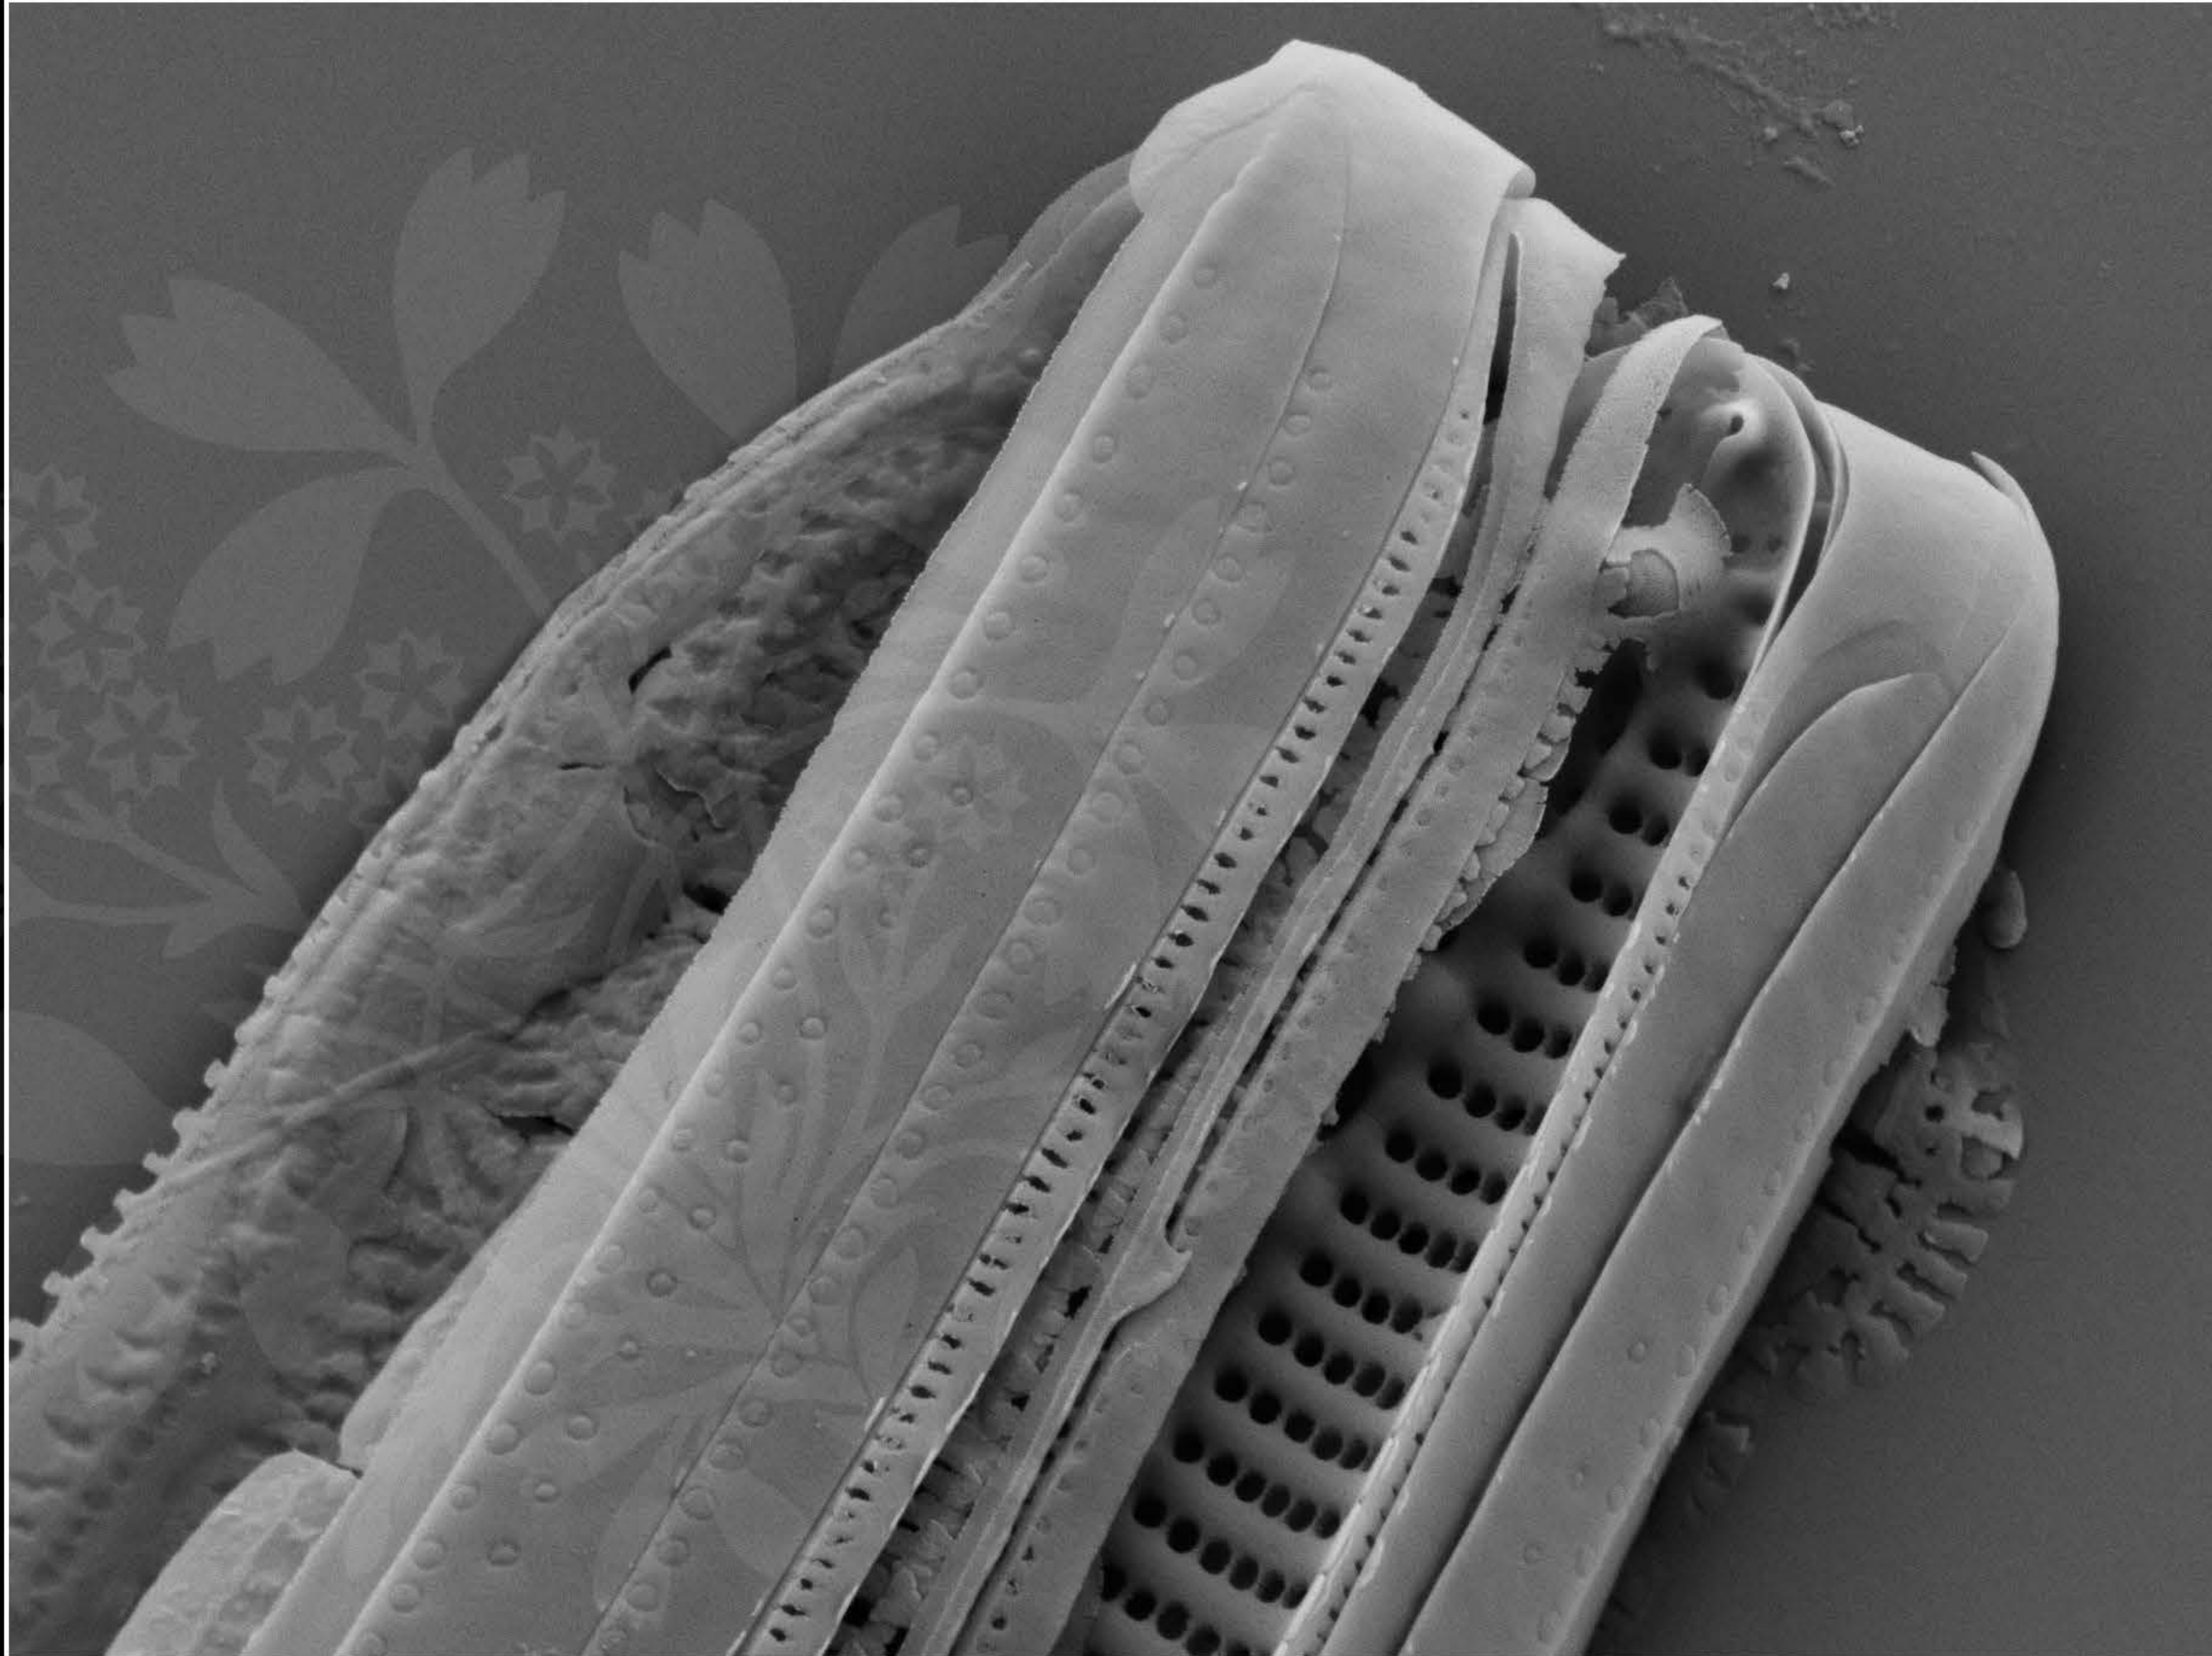

1 μ m

Mag = 20.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_09.tif



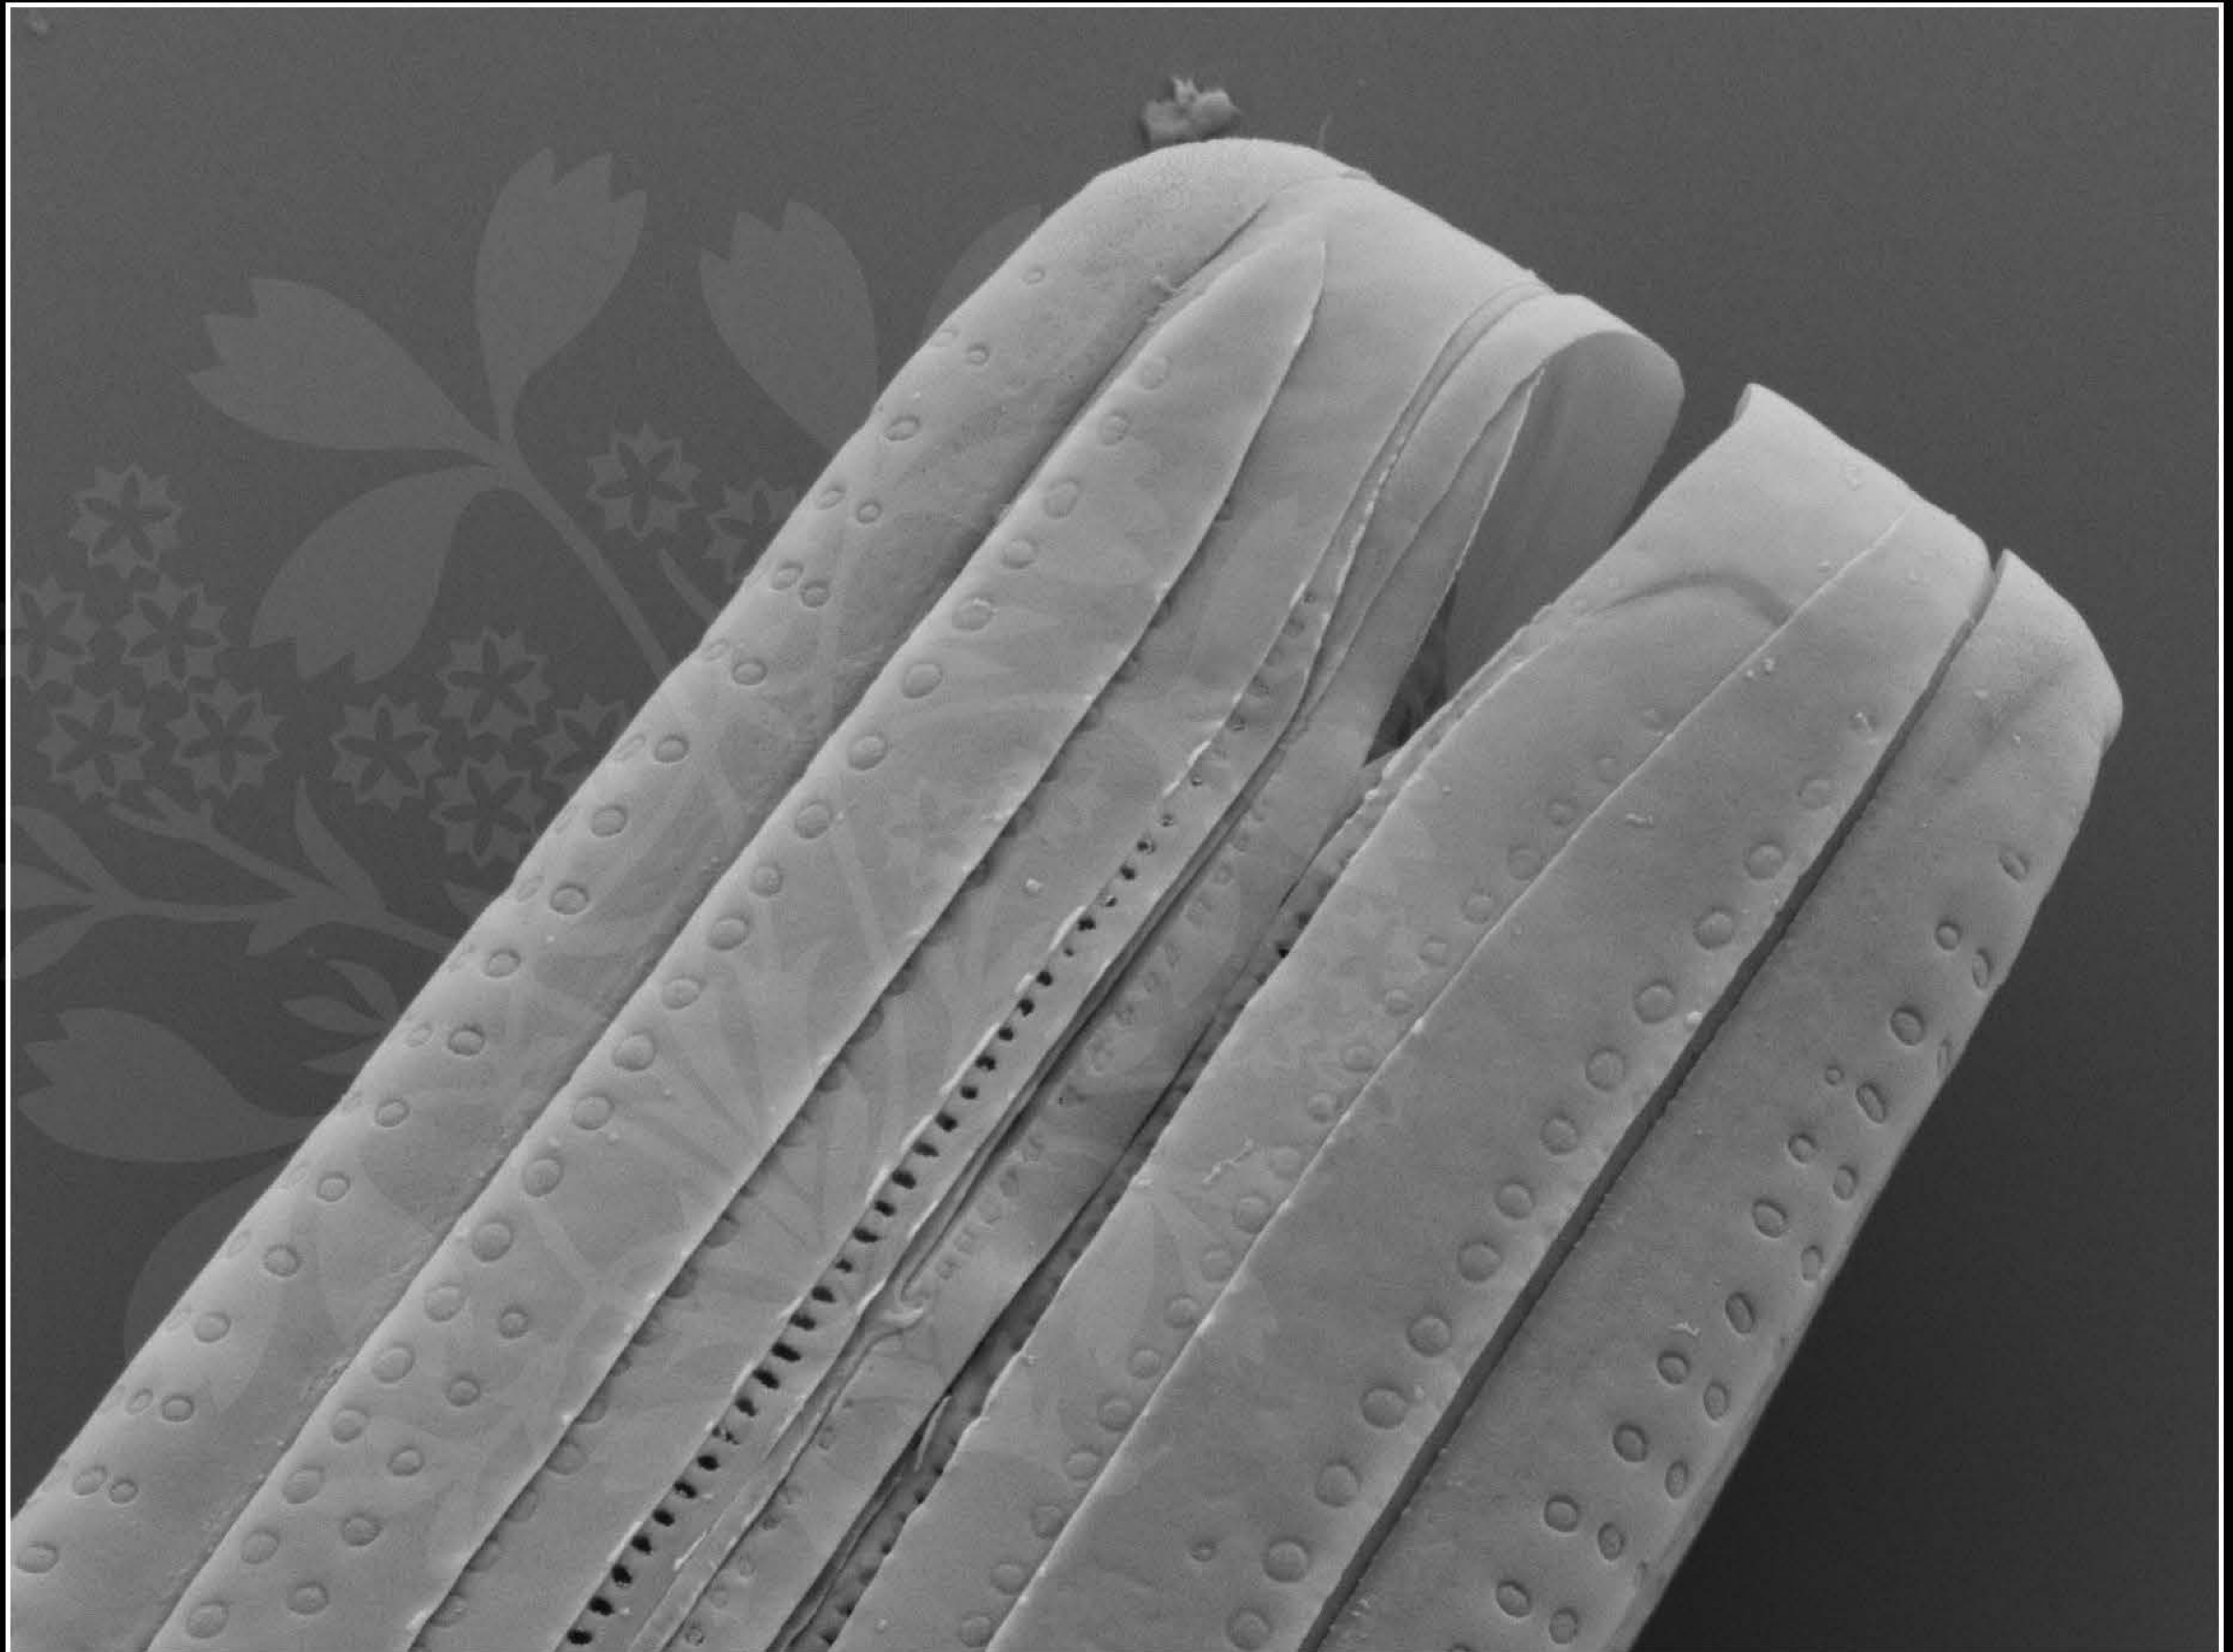

300 nm
└───┘

Mag = 25.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_10.tif



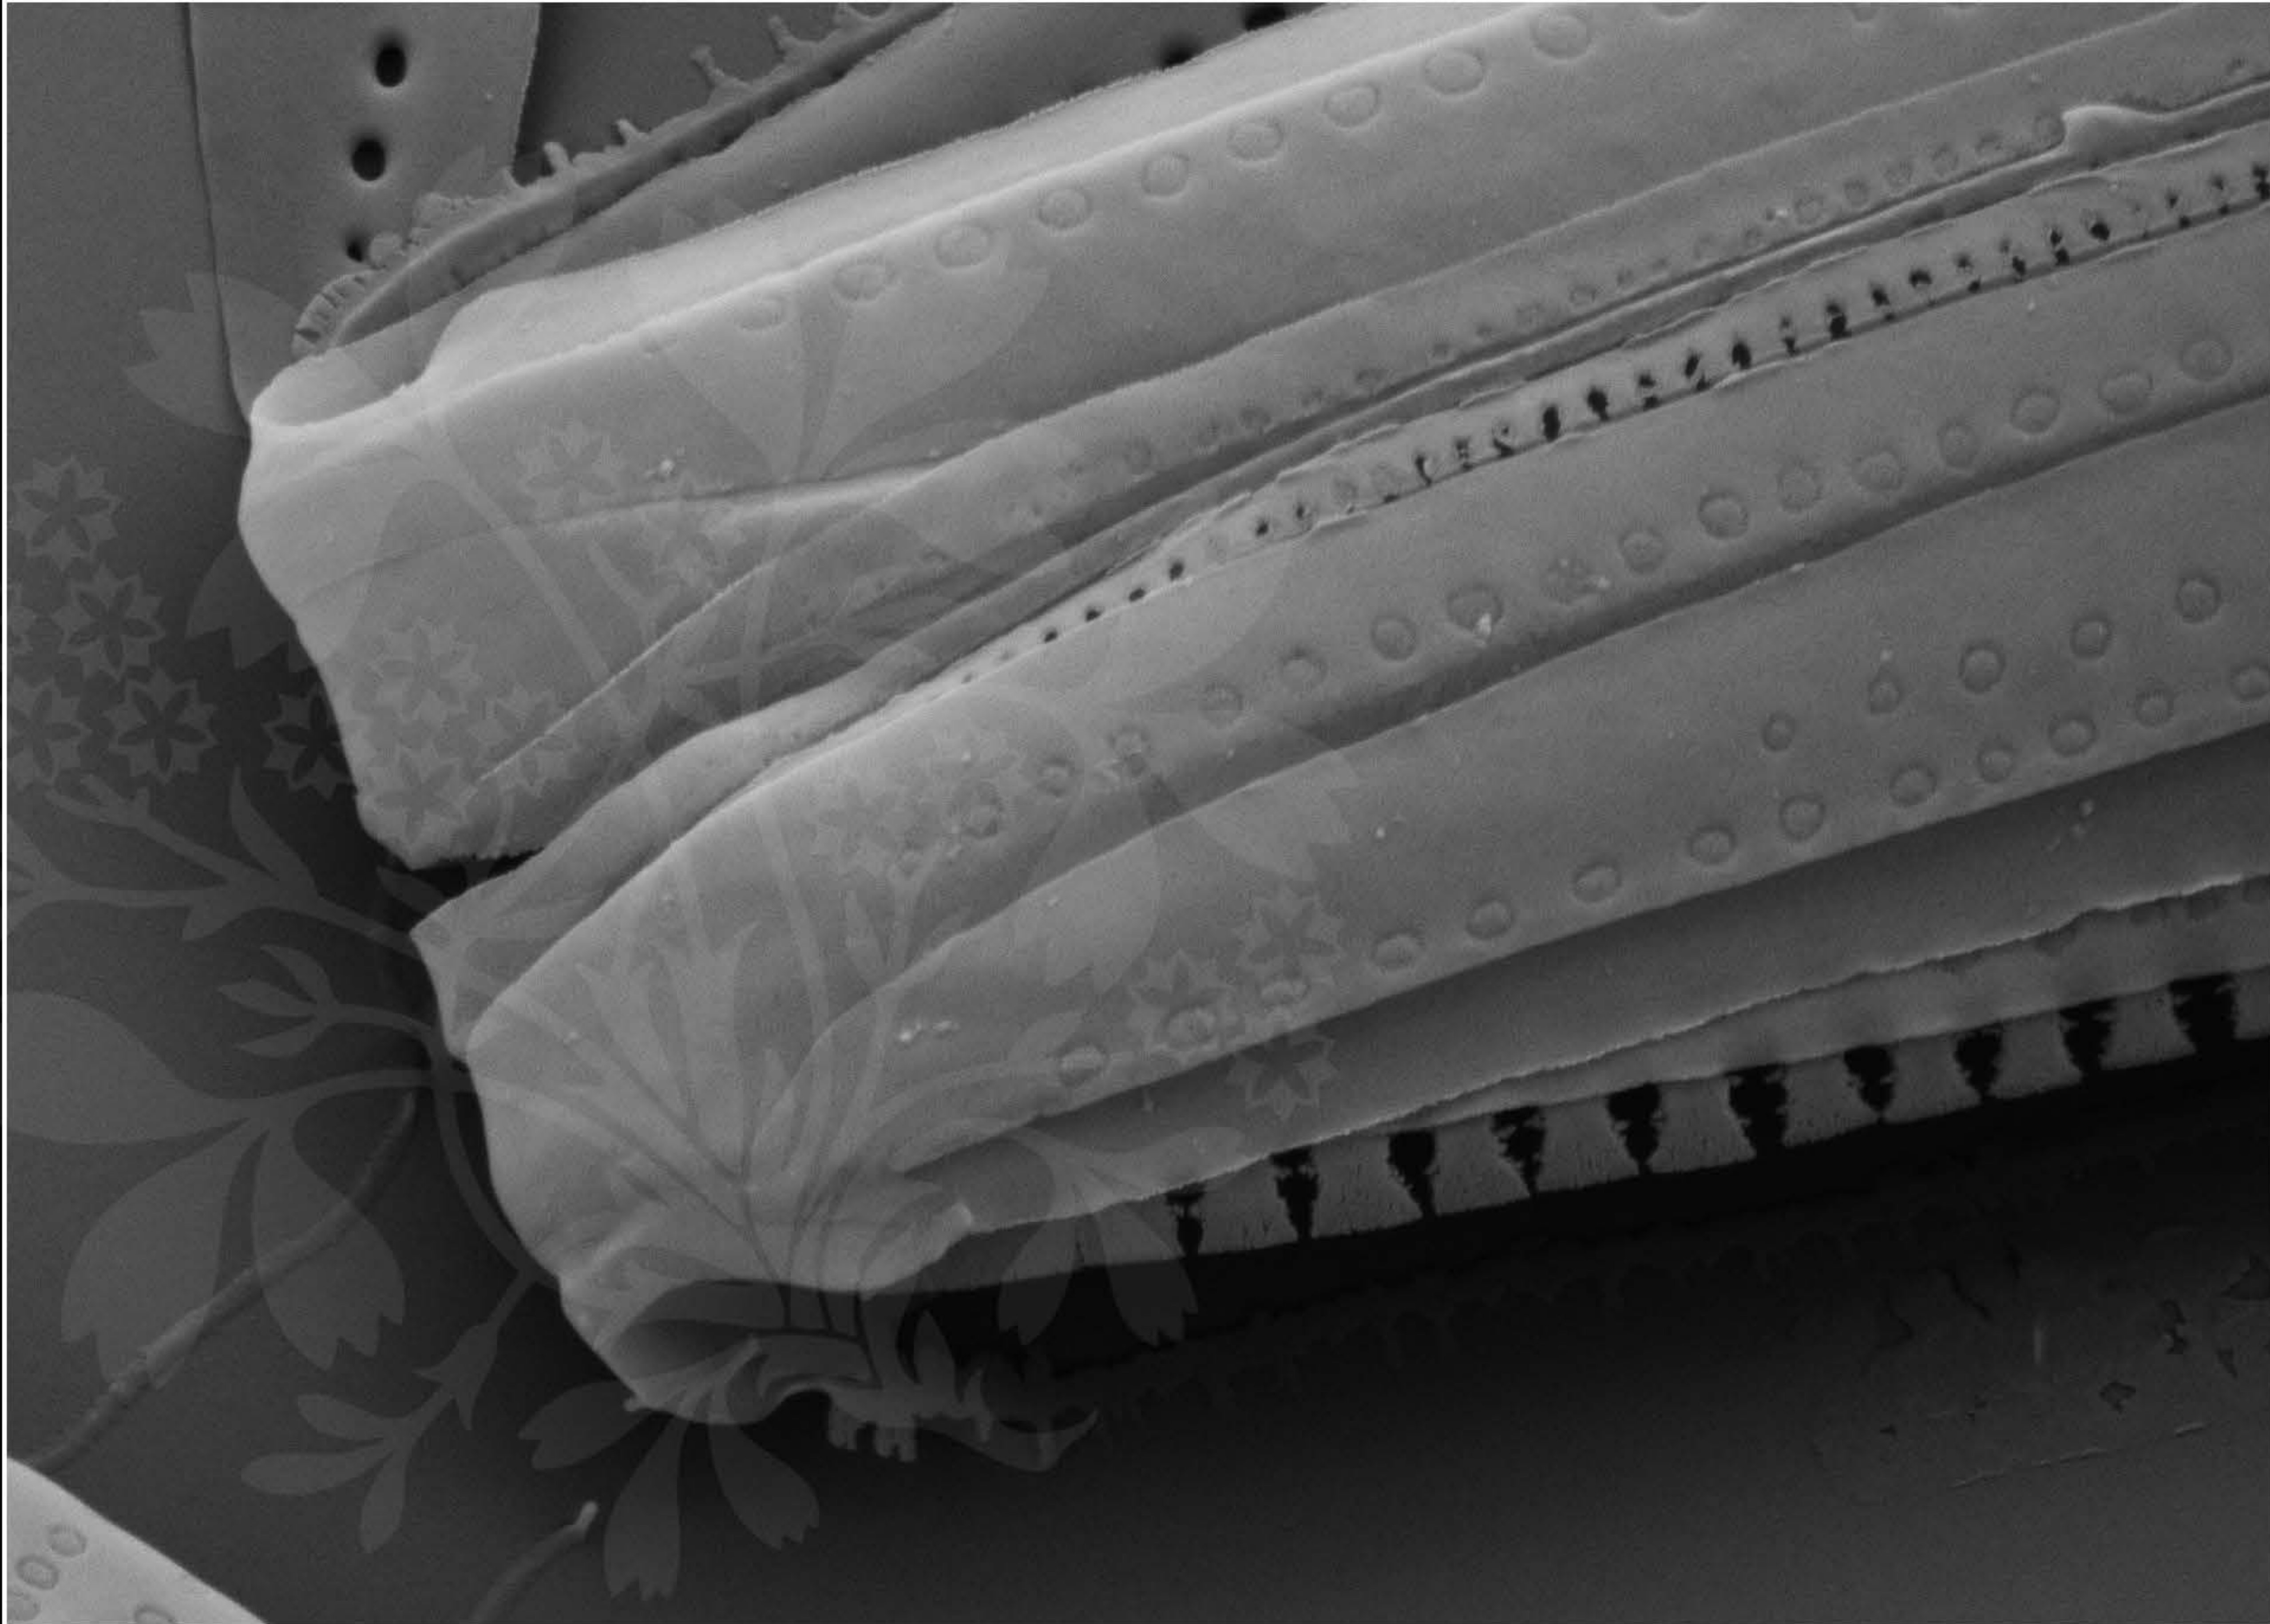

200 nm
┆

Mag = 30.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_11.tif



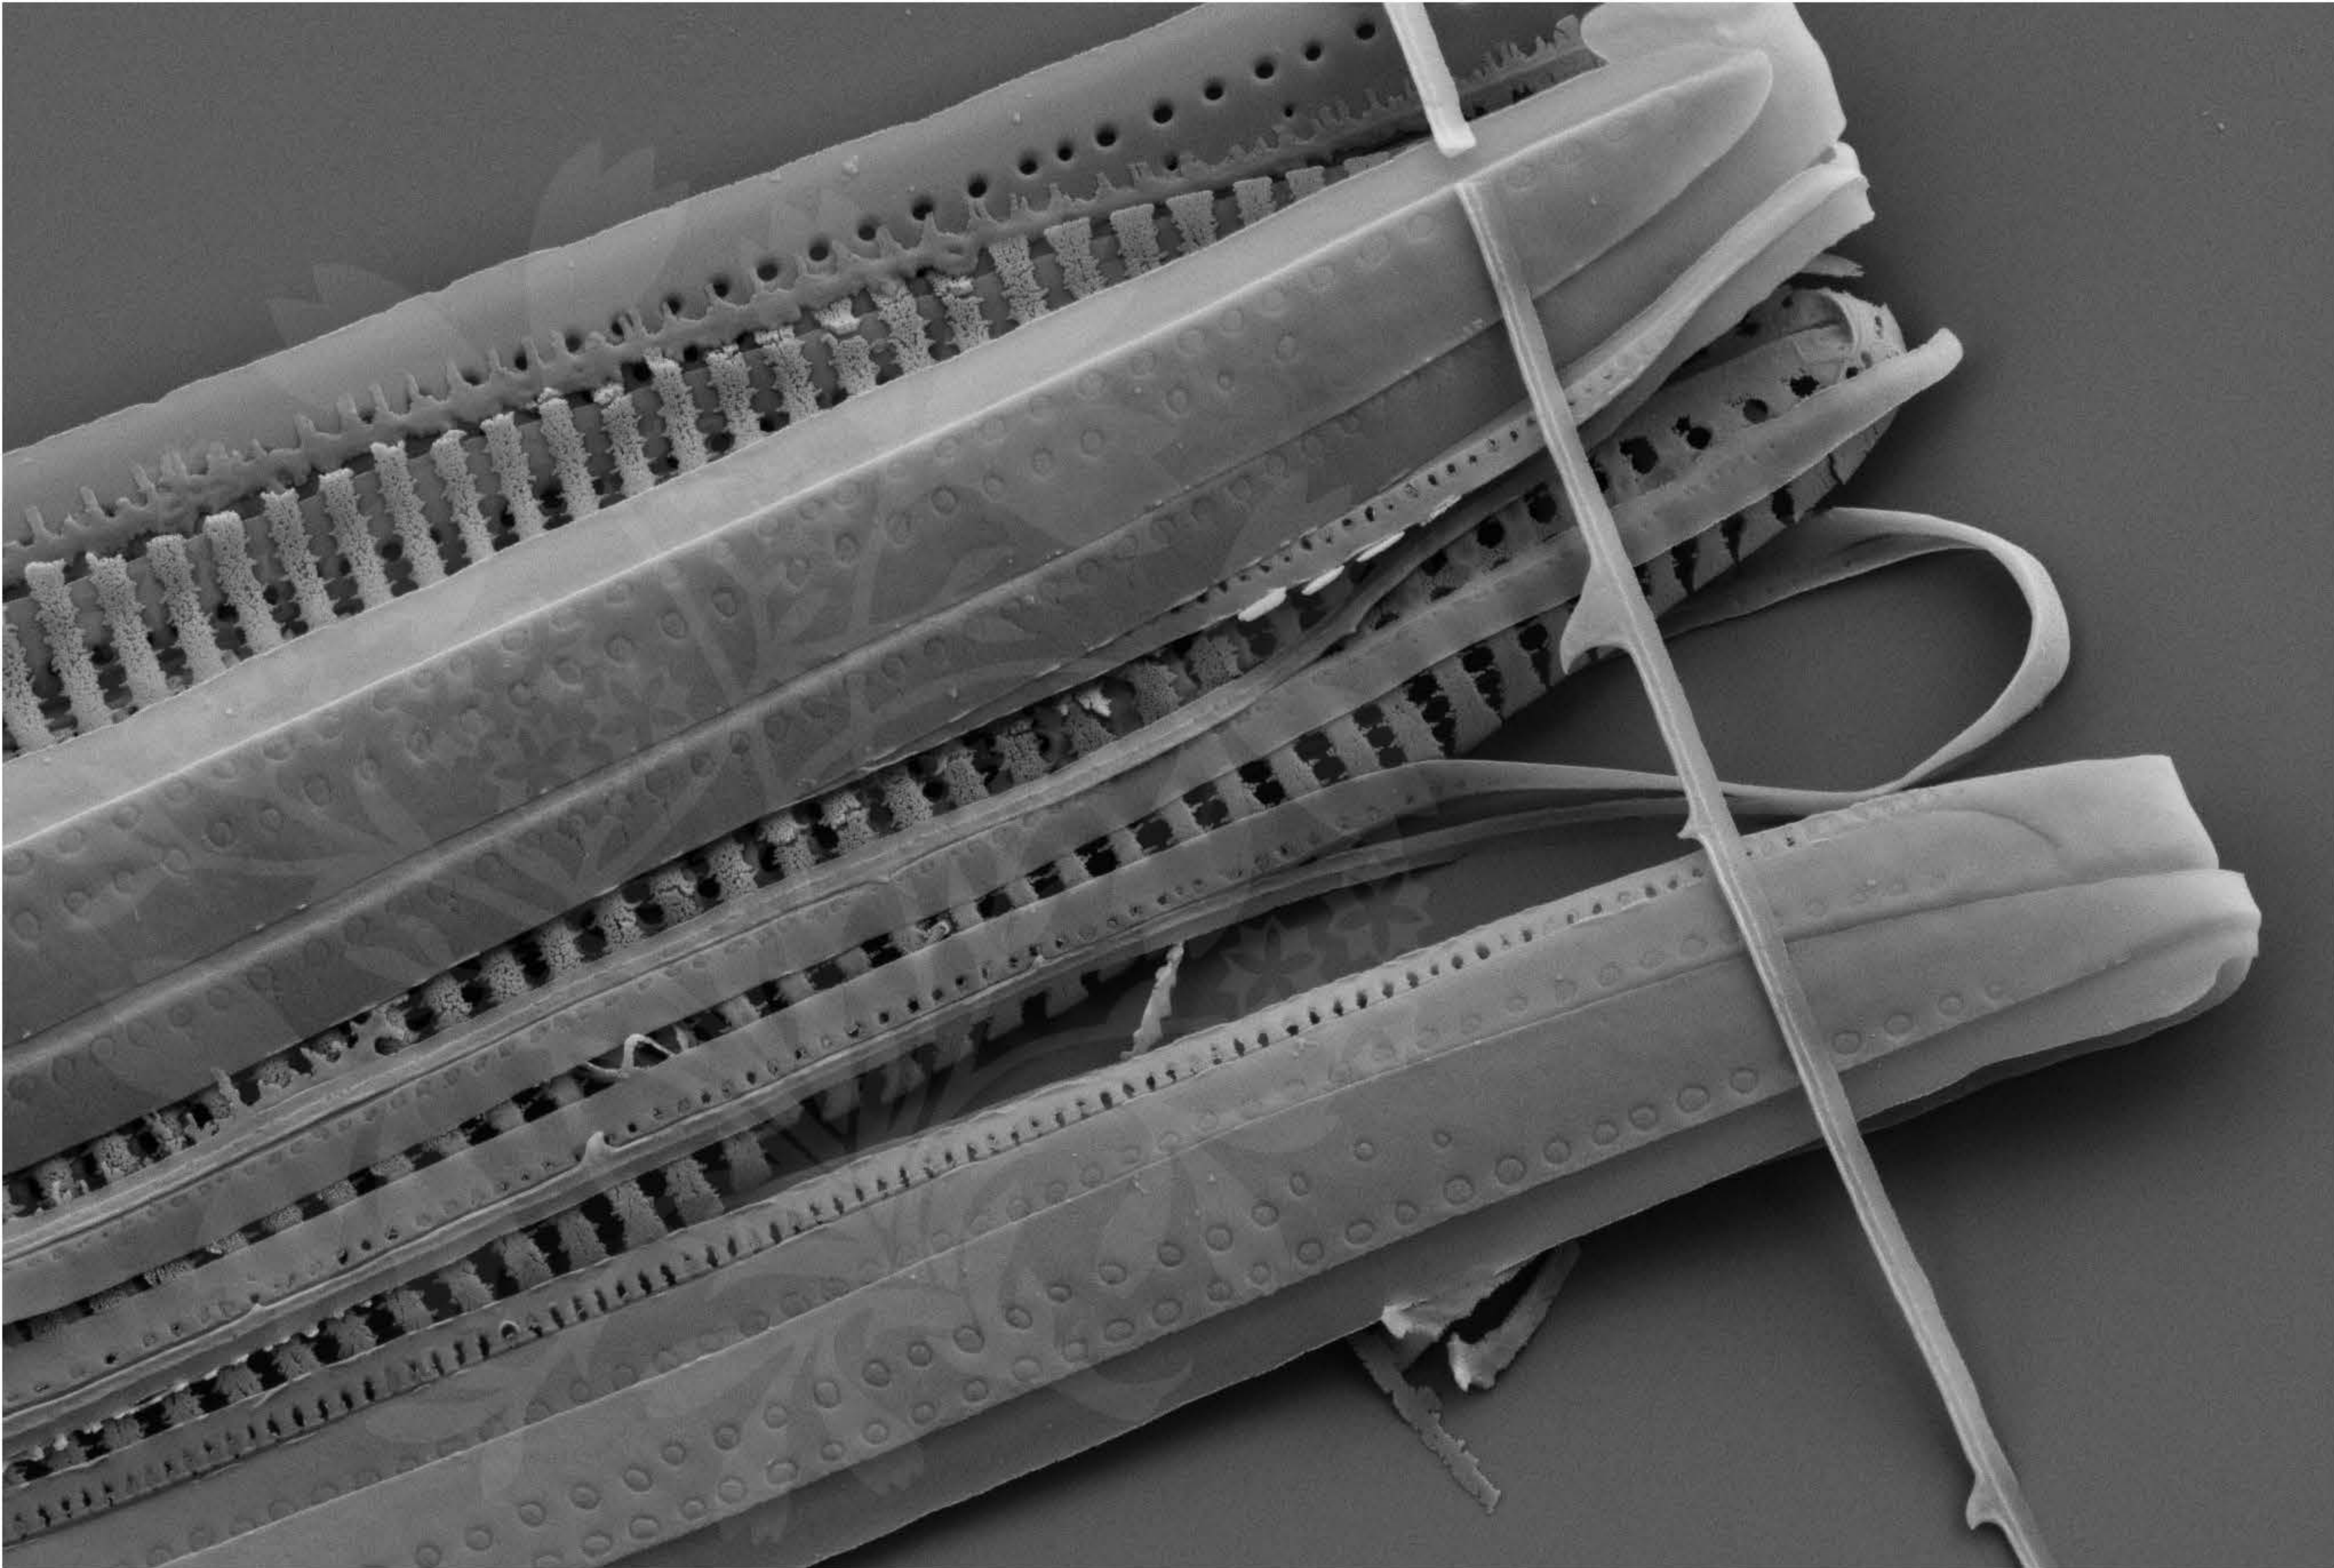

1 μm

Mag = 16.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_12.tif



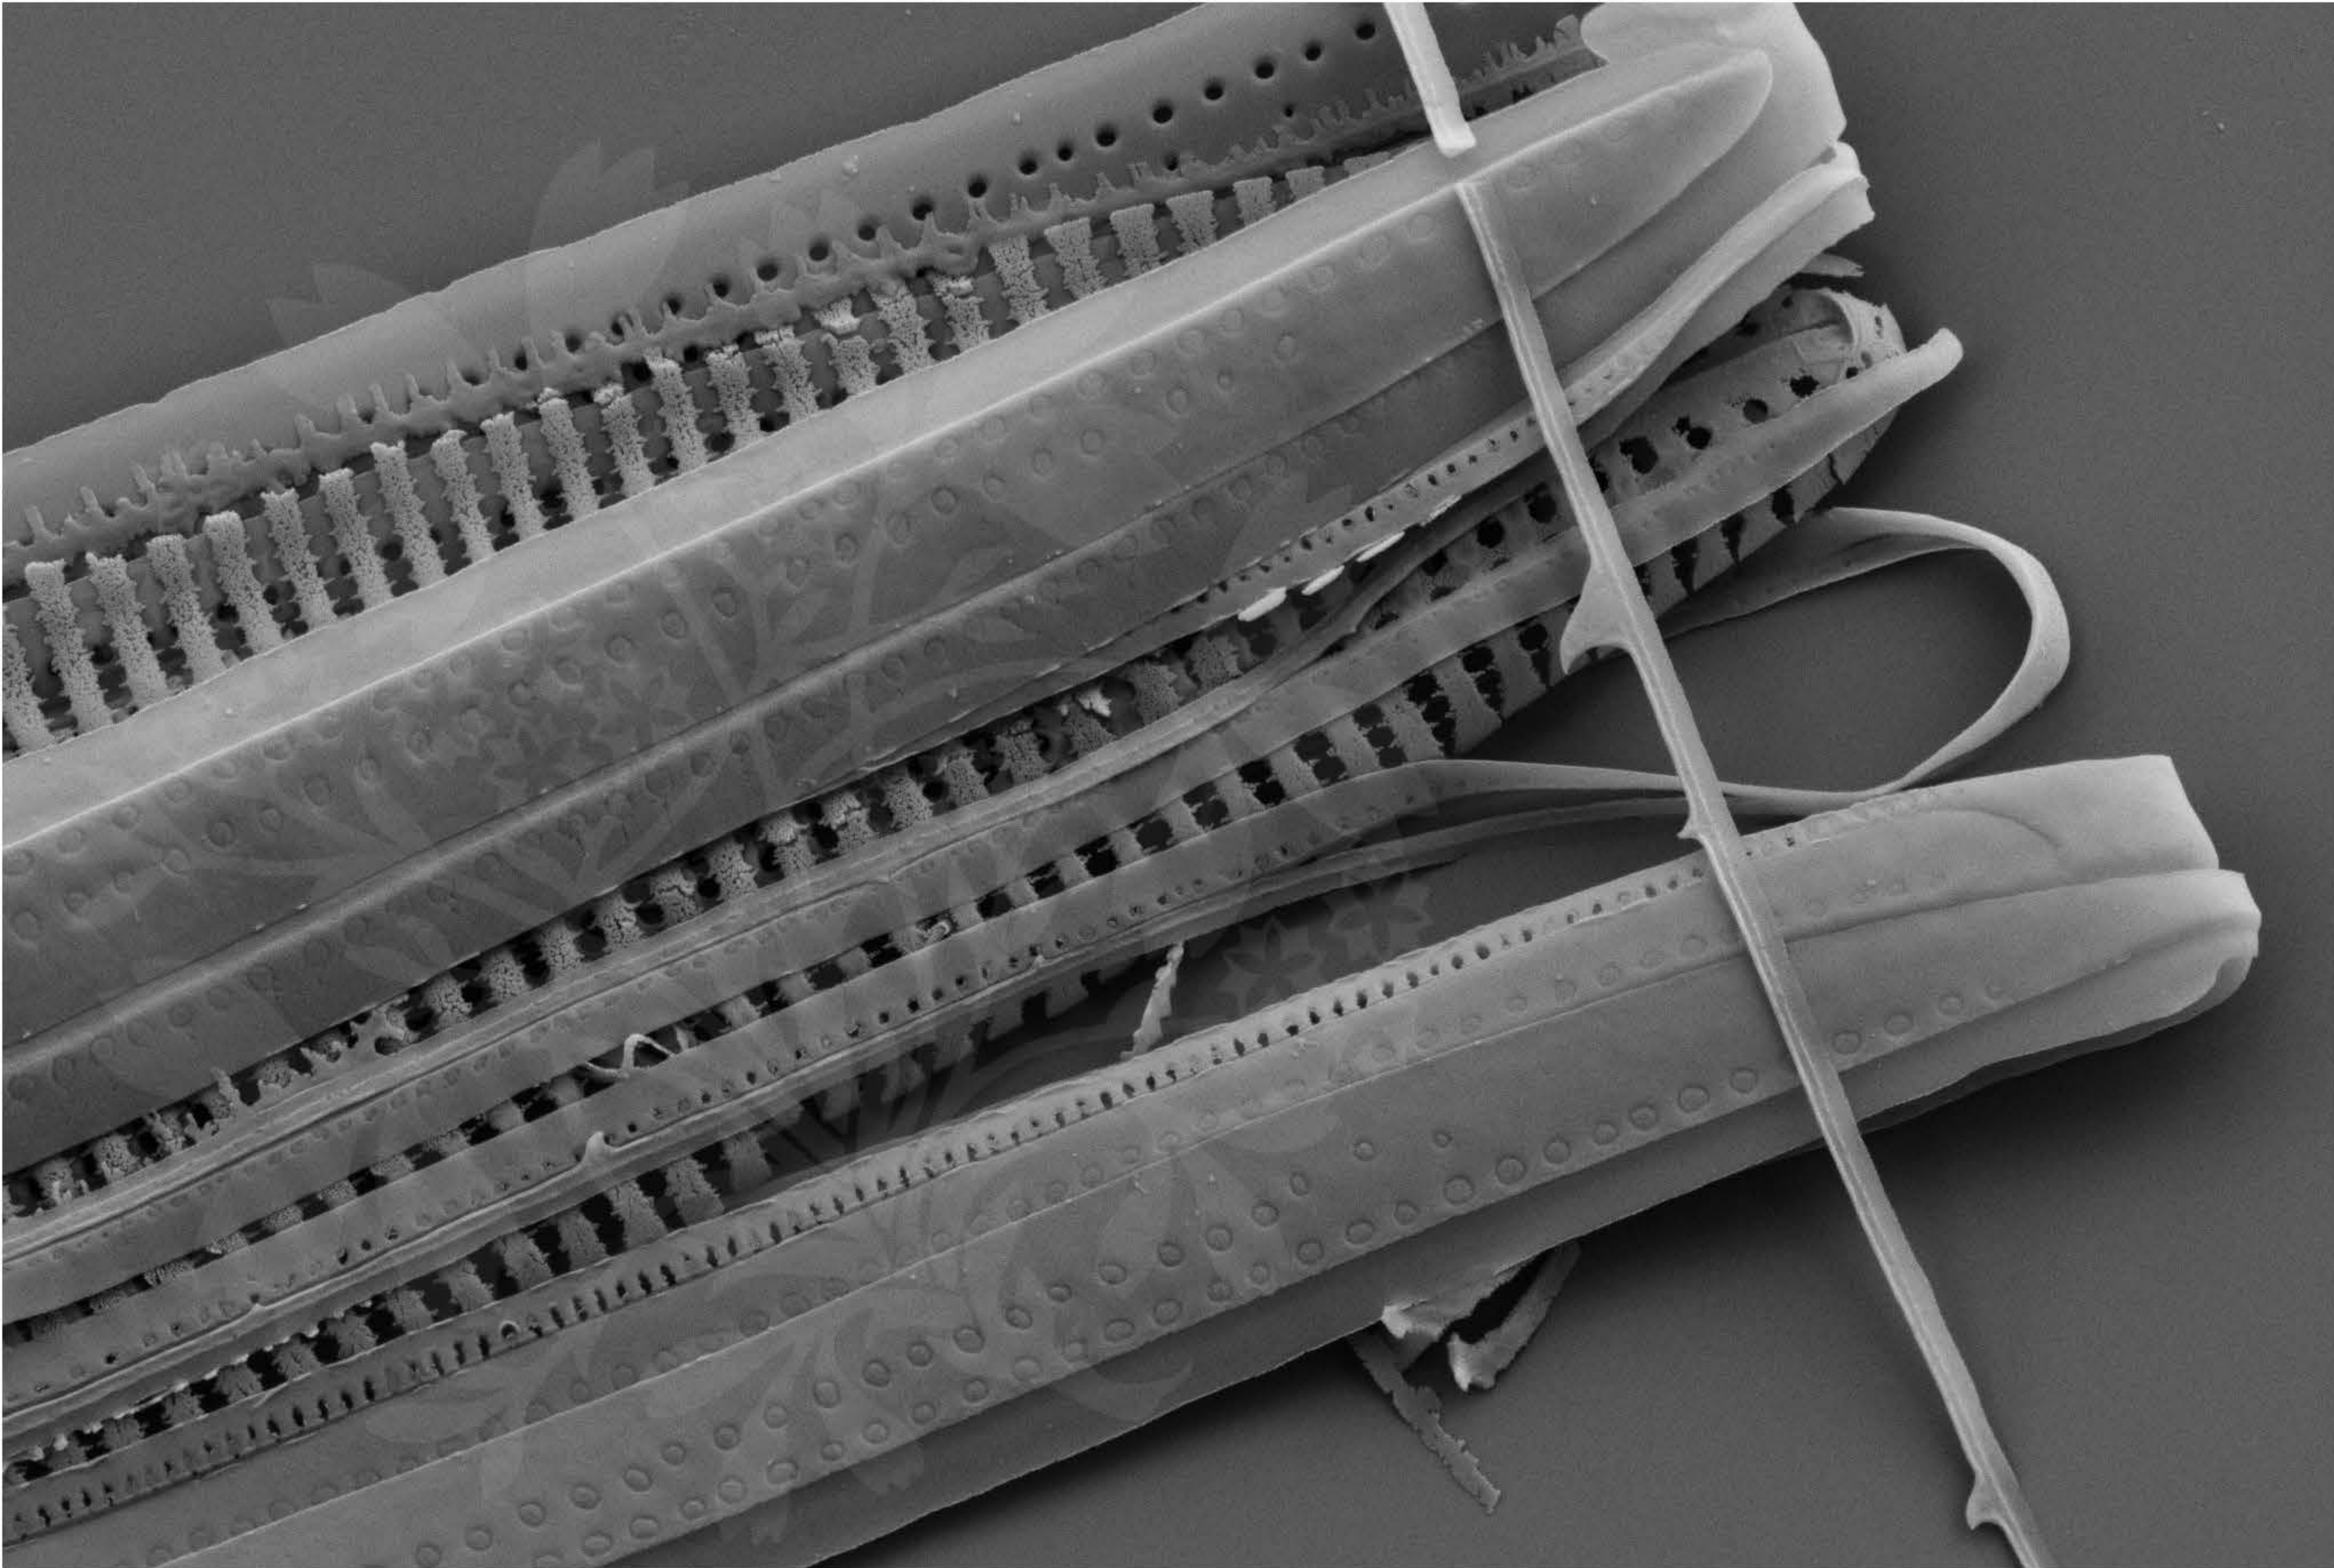

1 μm

Mag = 16.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_13.tif



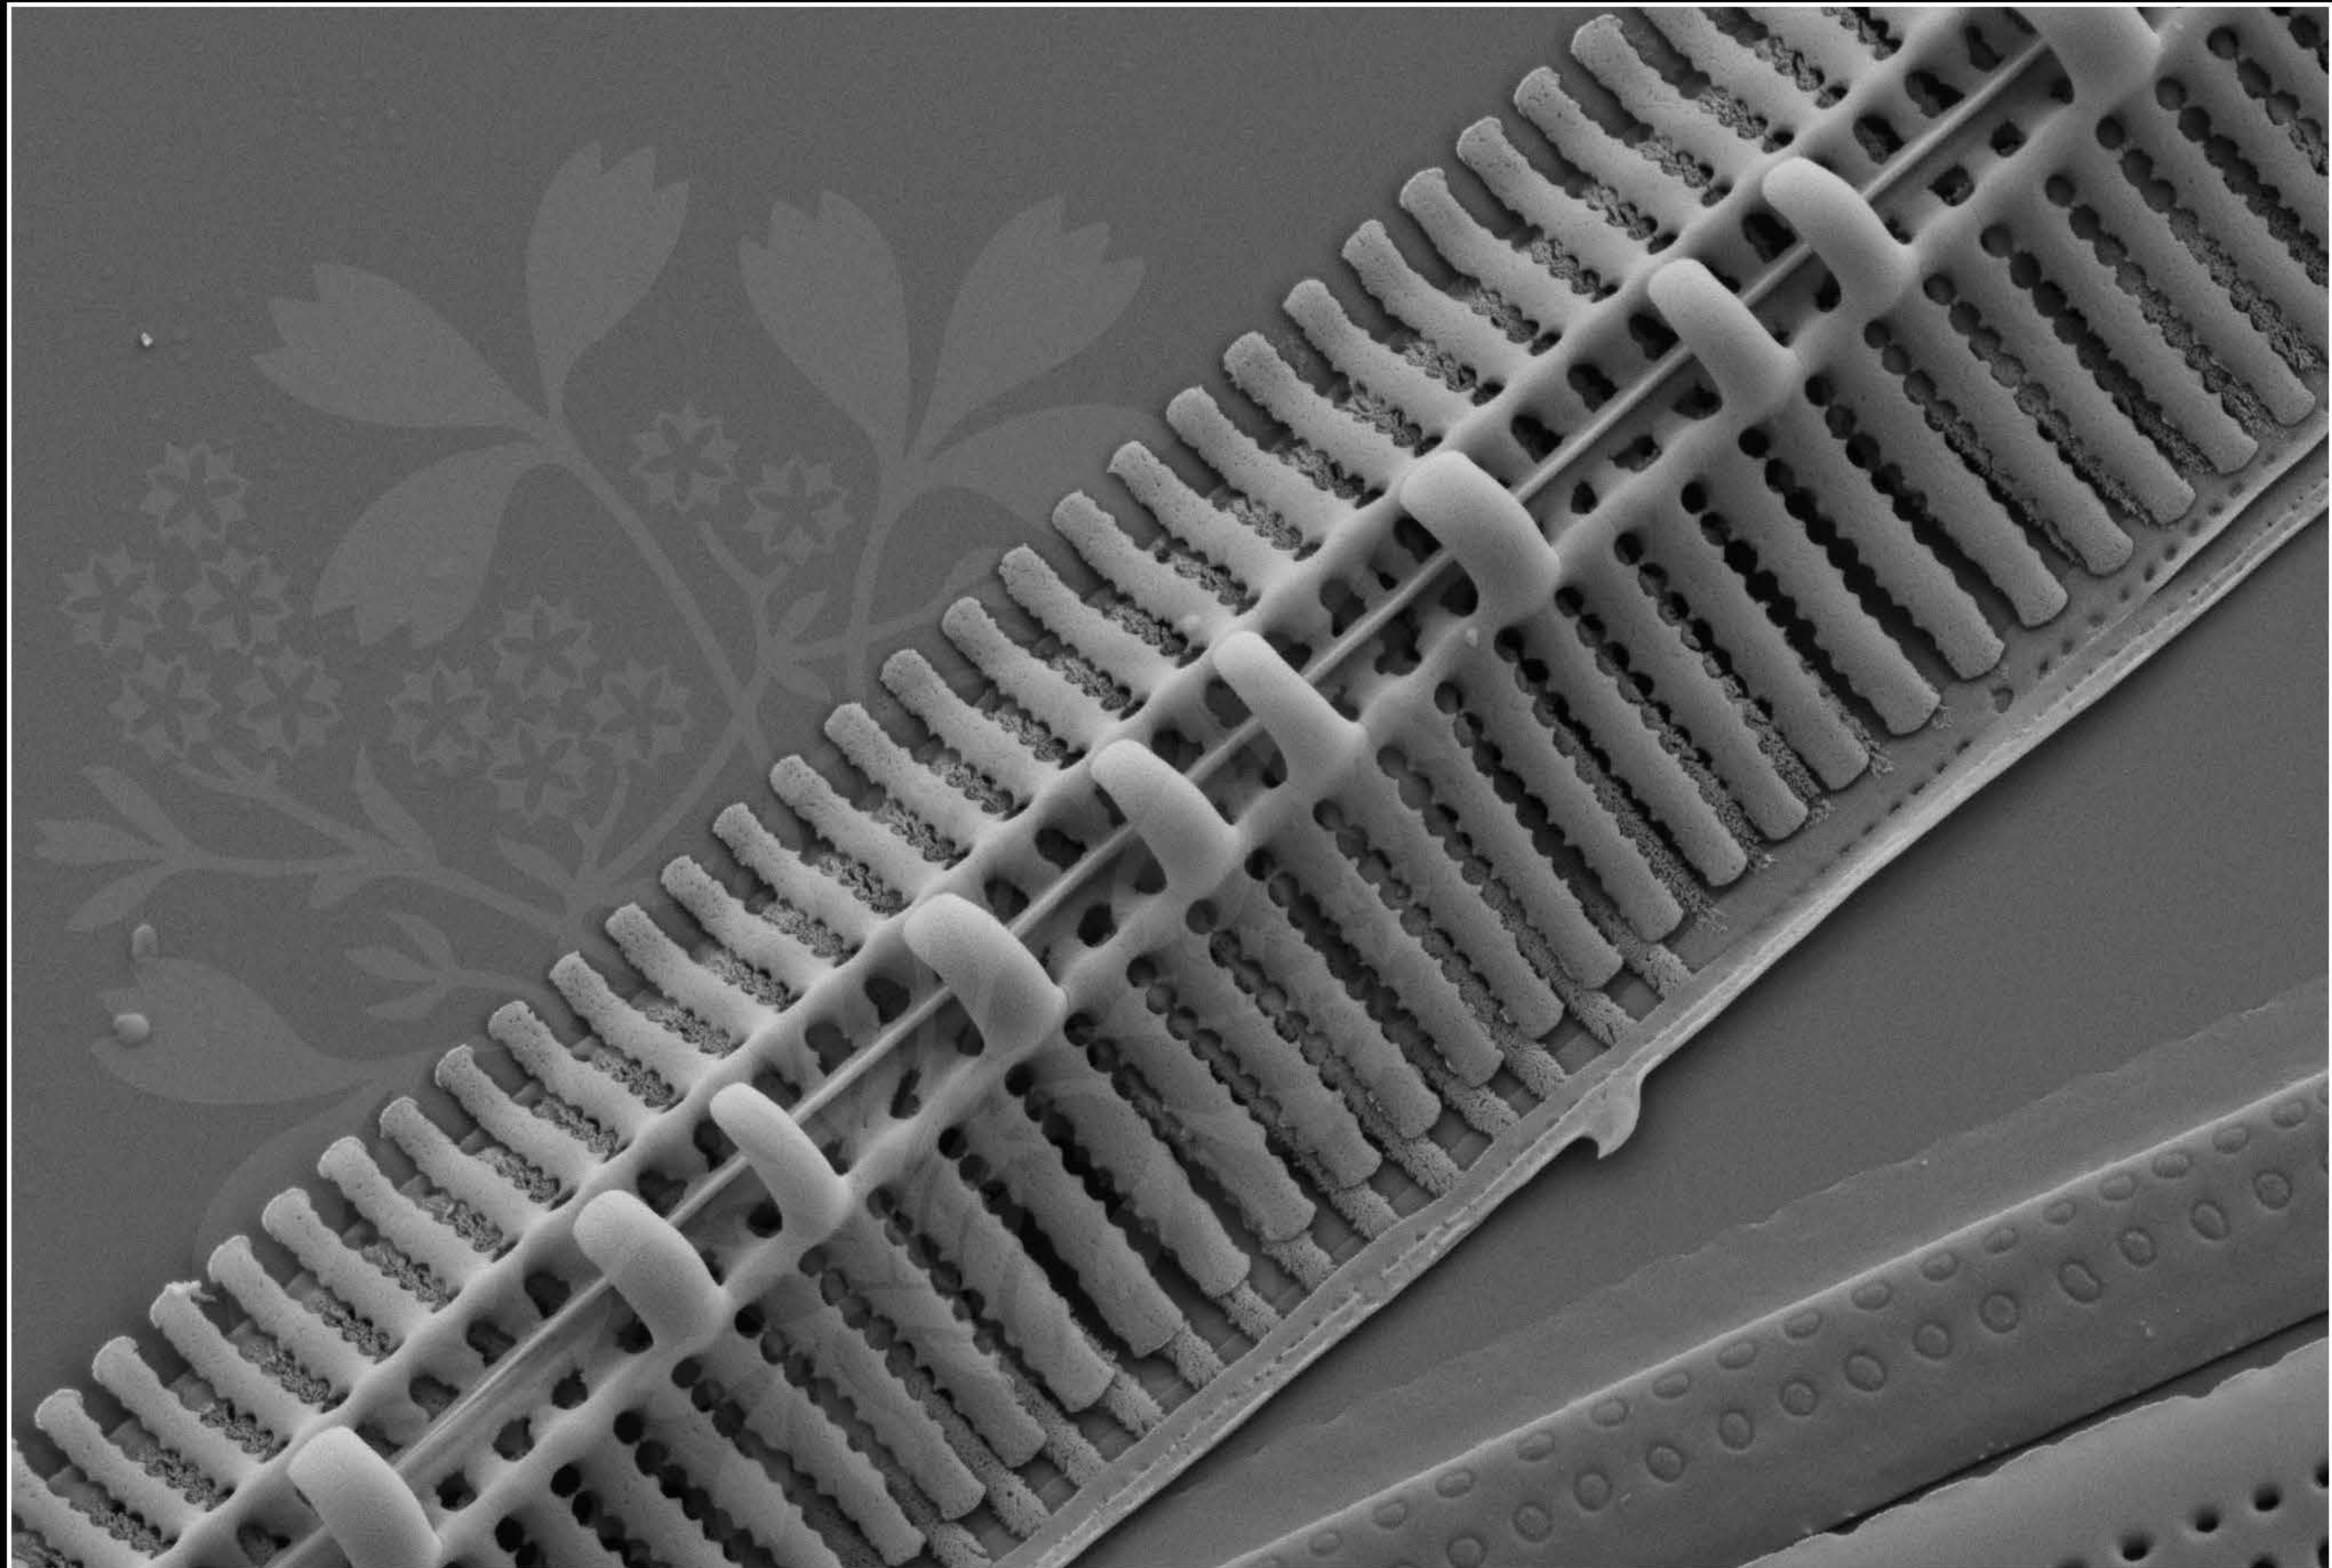

1 μm

Mag = 20.00 K X

EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_14.tif





1 μm

Mag = 16.00 K X

EHT = 4.50 kV


Signal A = SE2

Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_15.tif



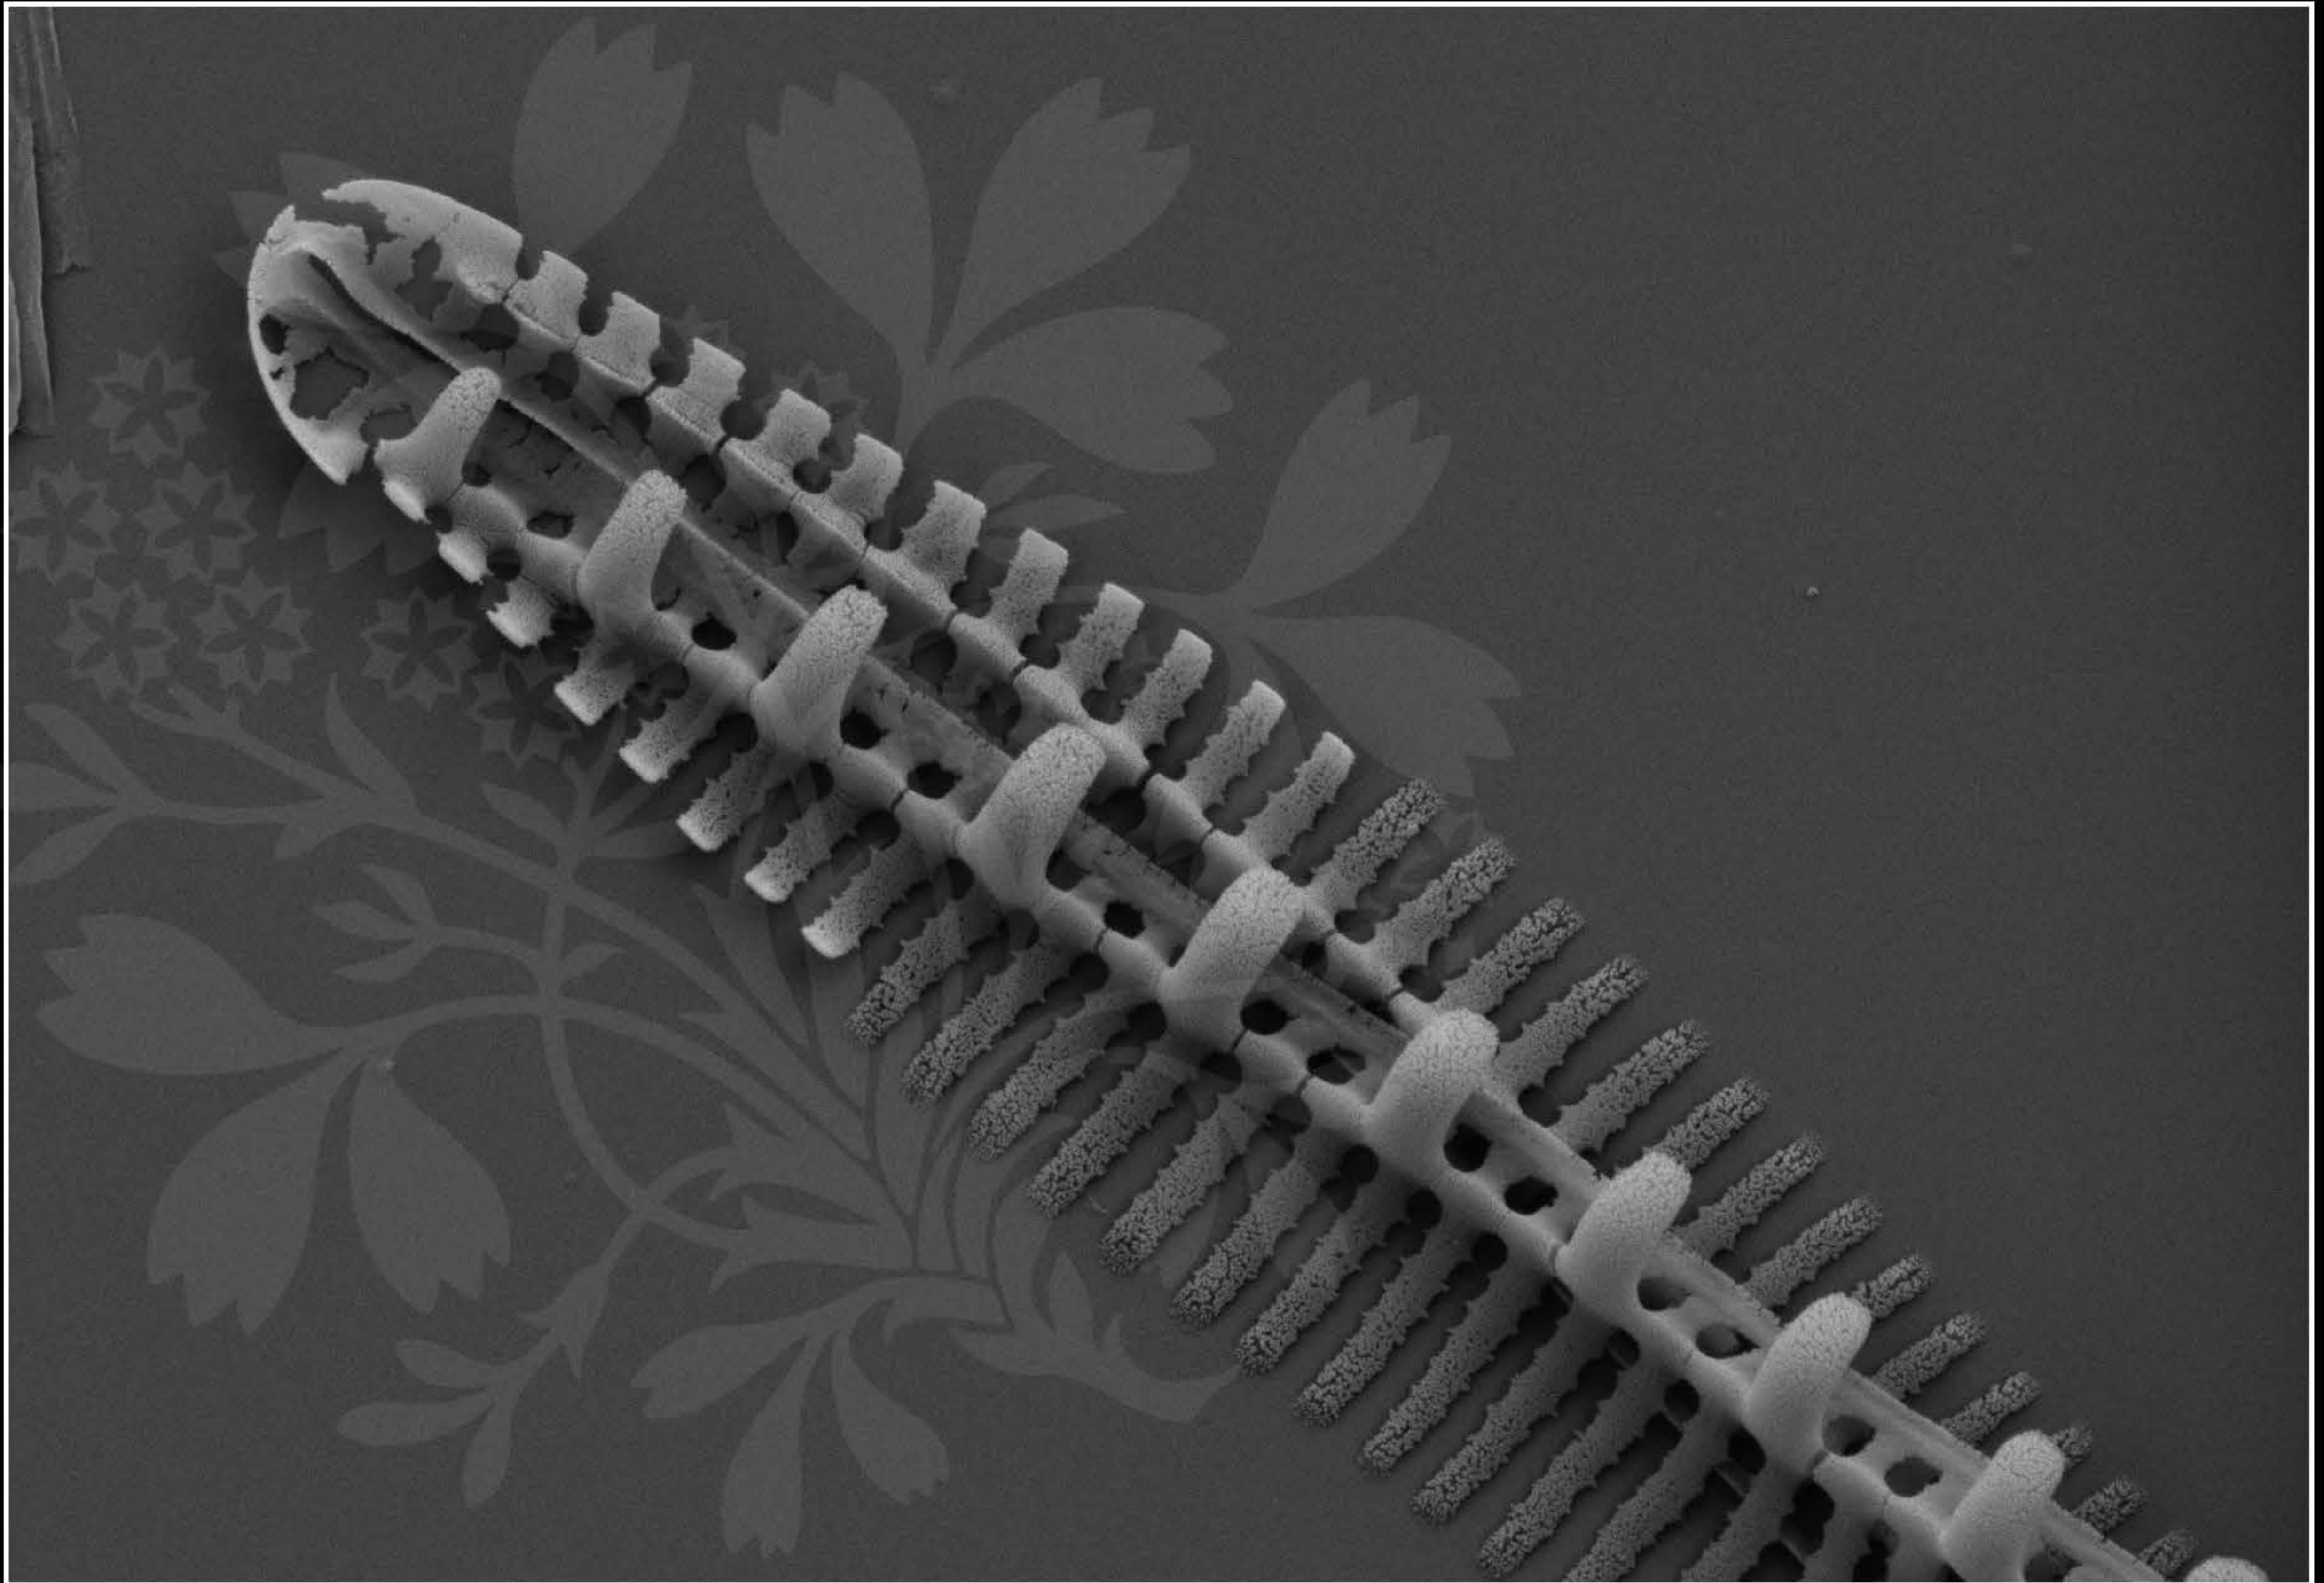

1 μm

Mag = 20.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_16.tif



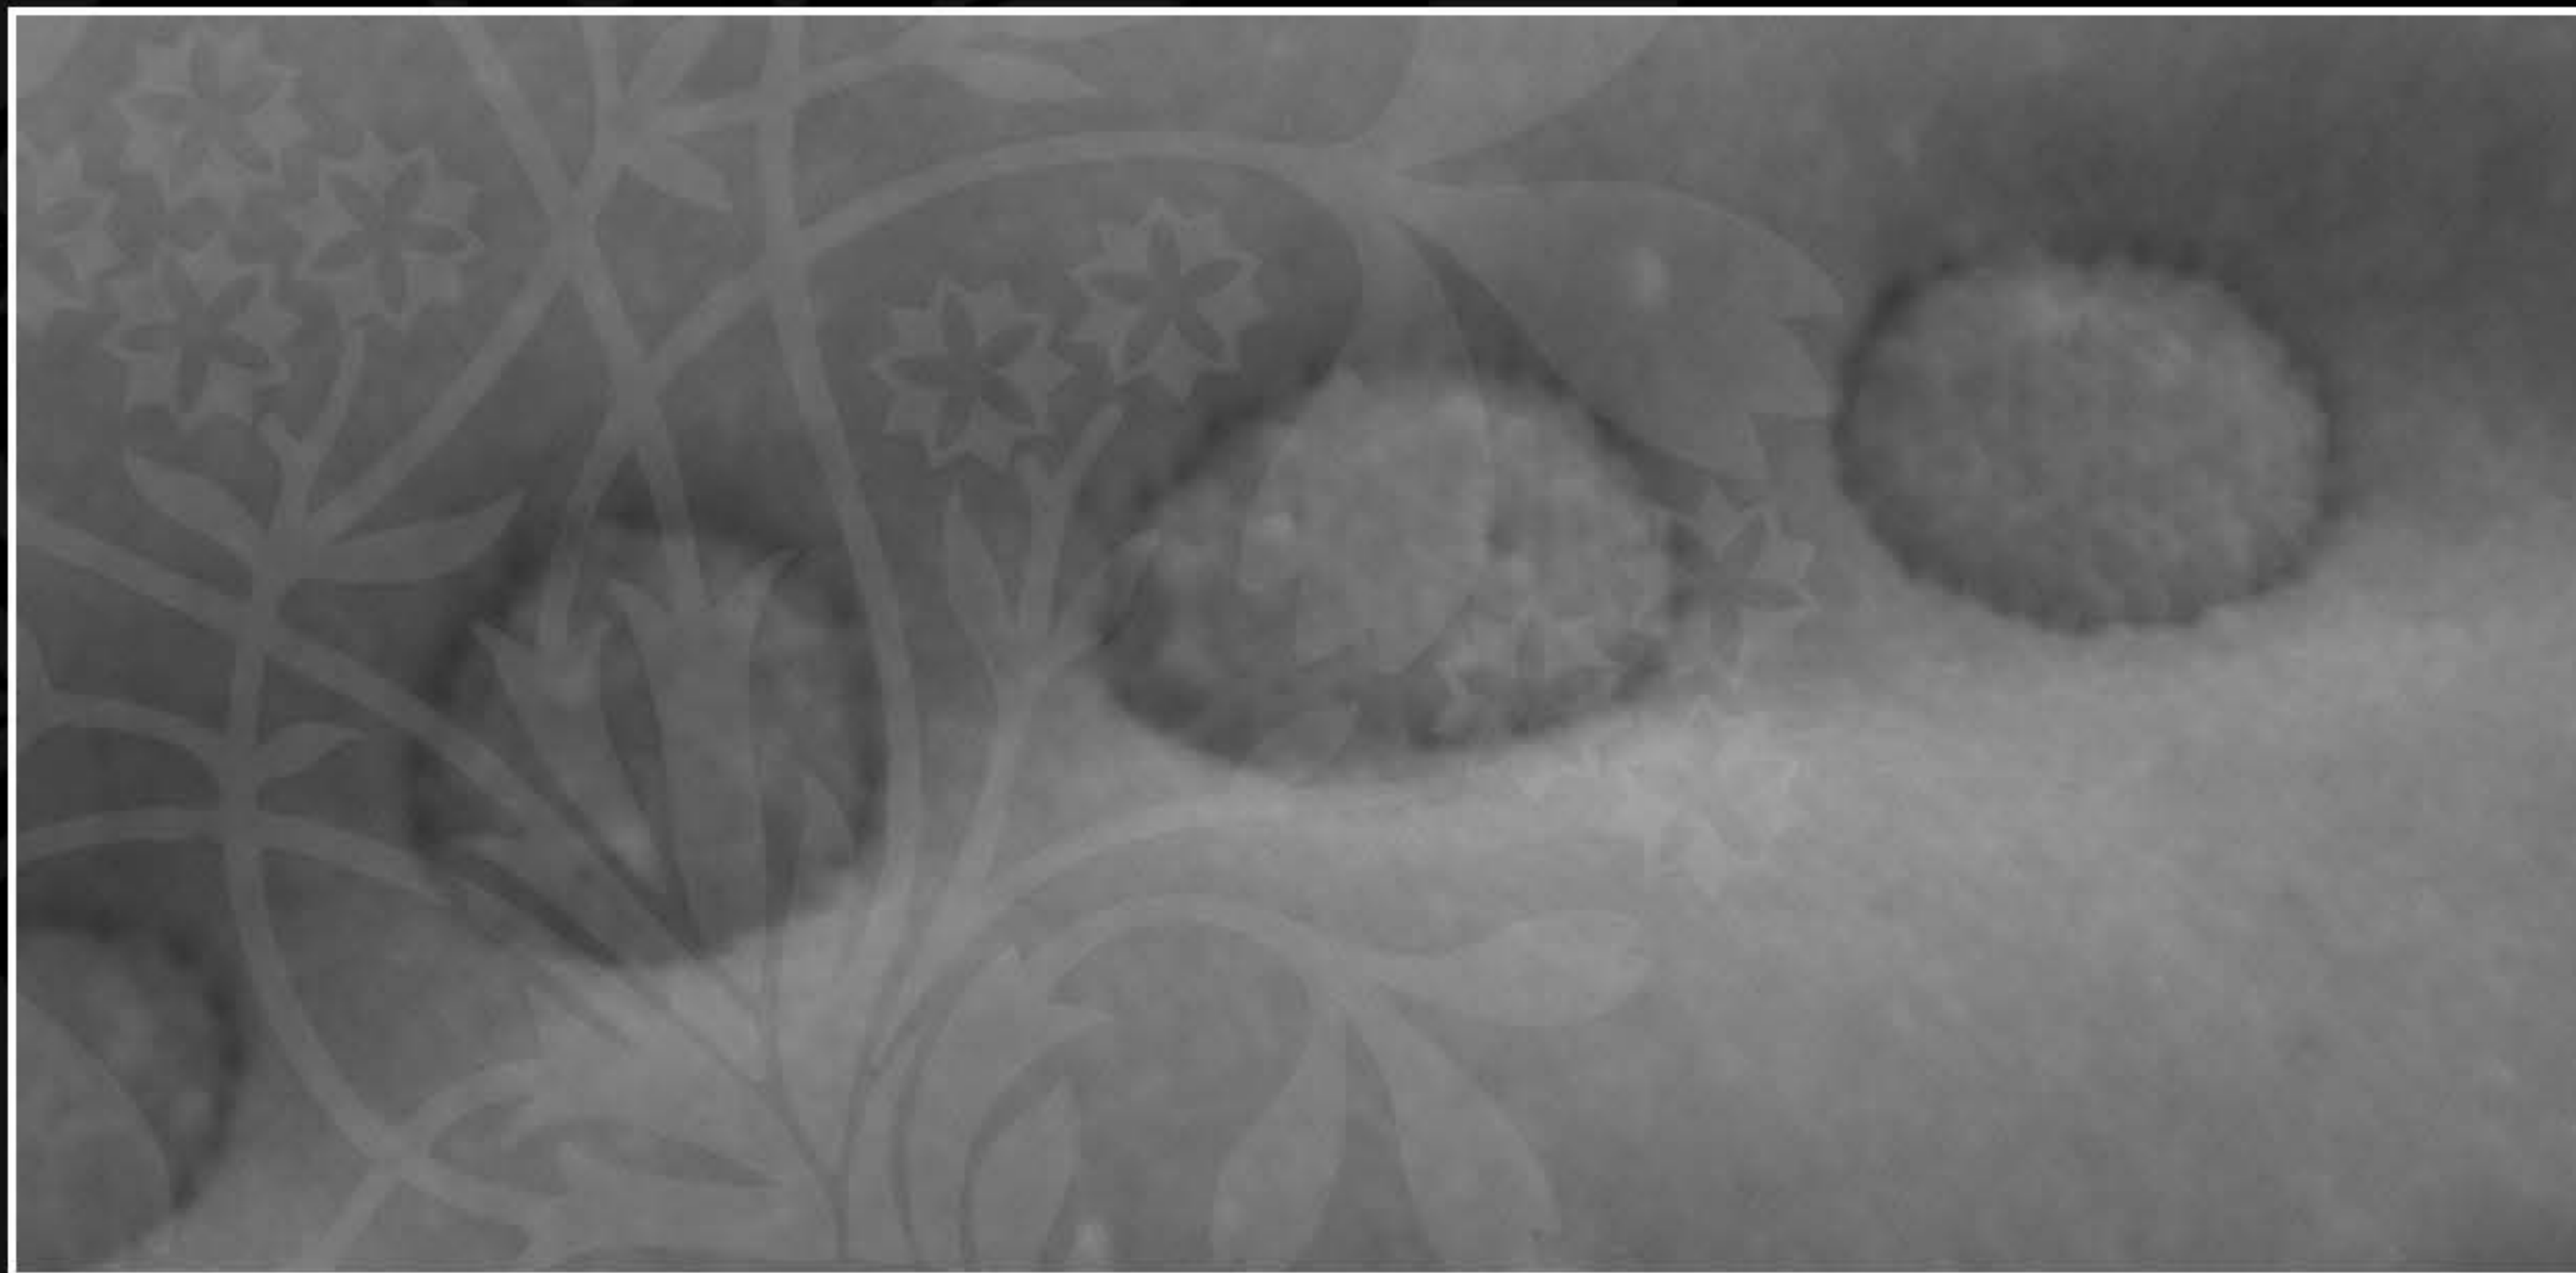

100 nm

Mag = 200.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_17.tif



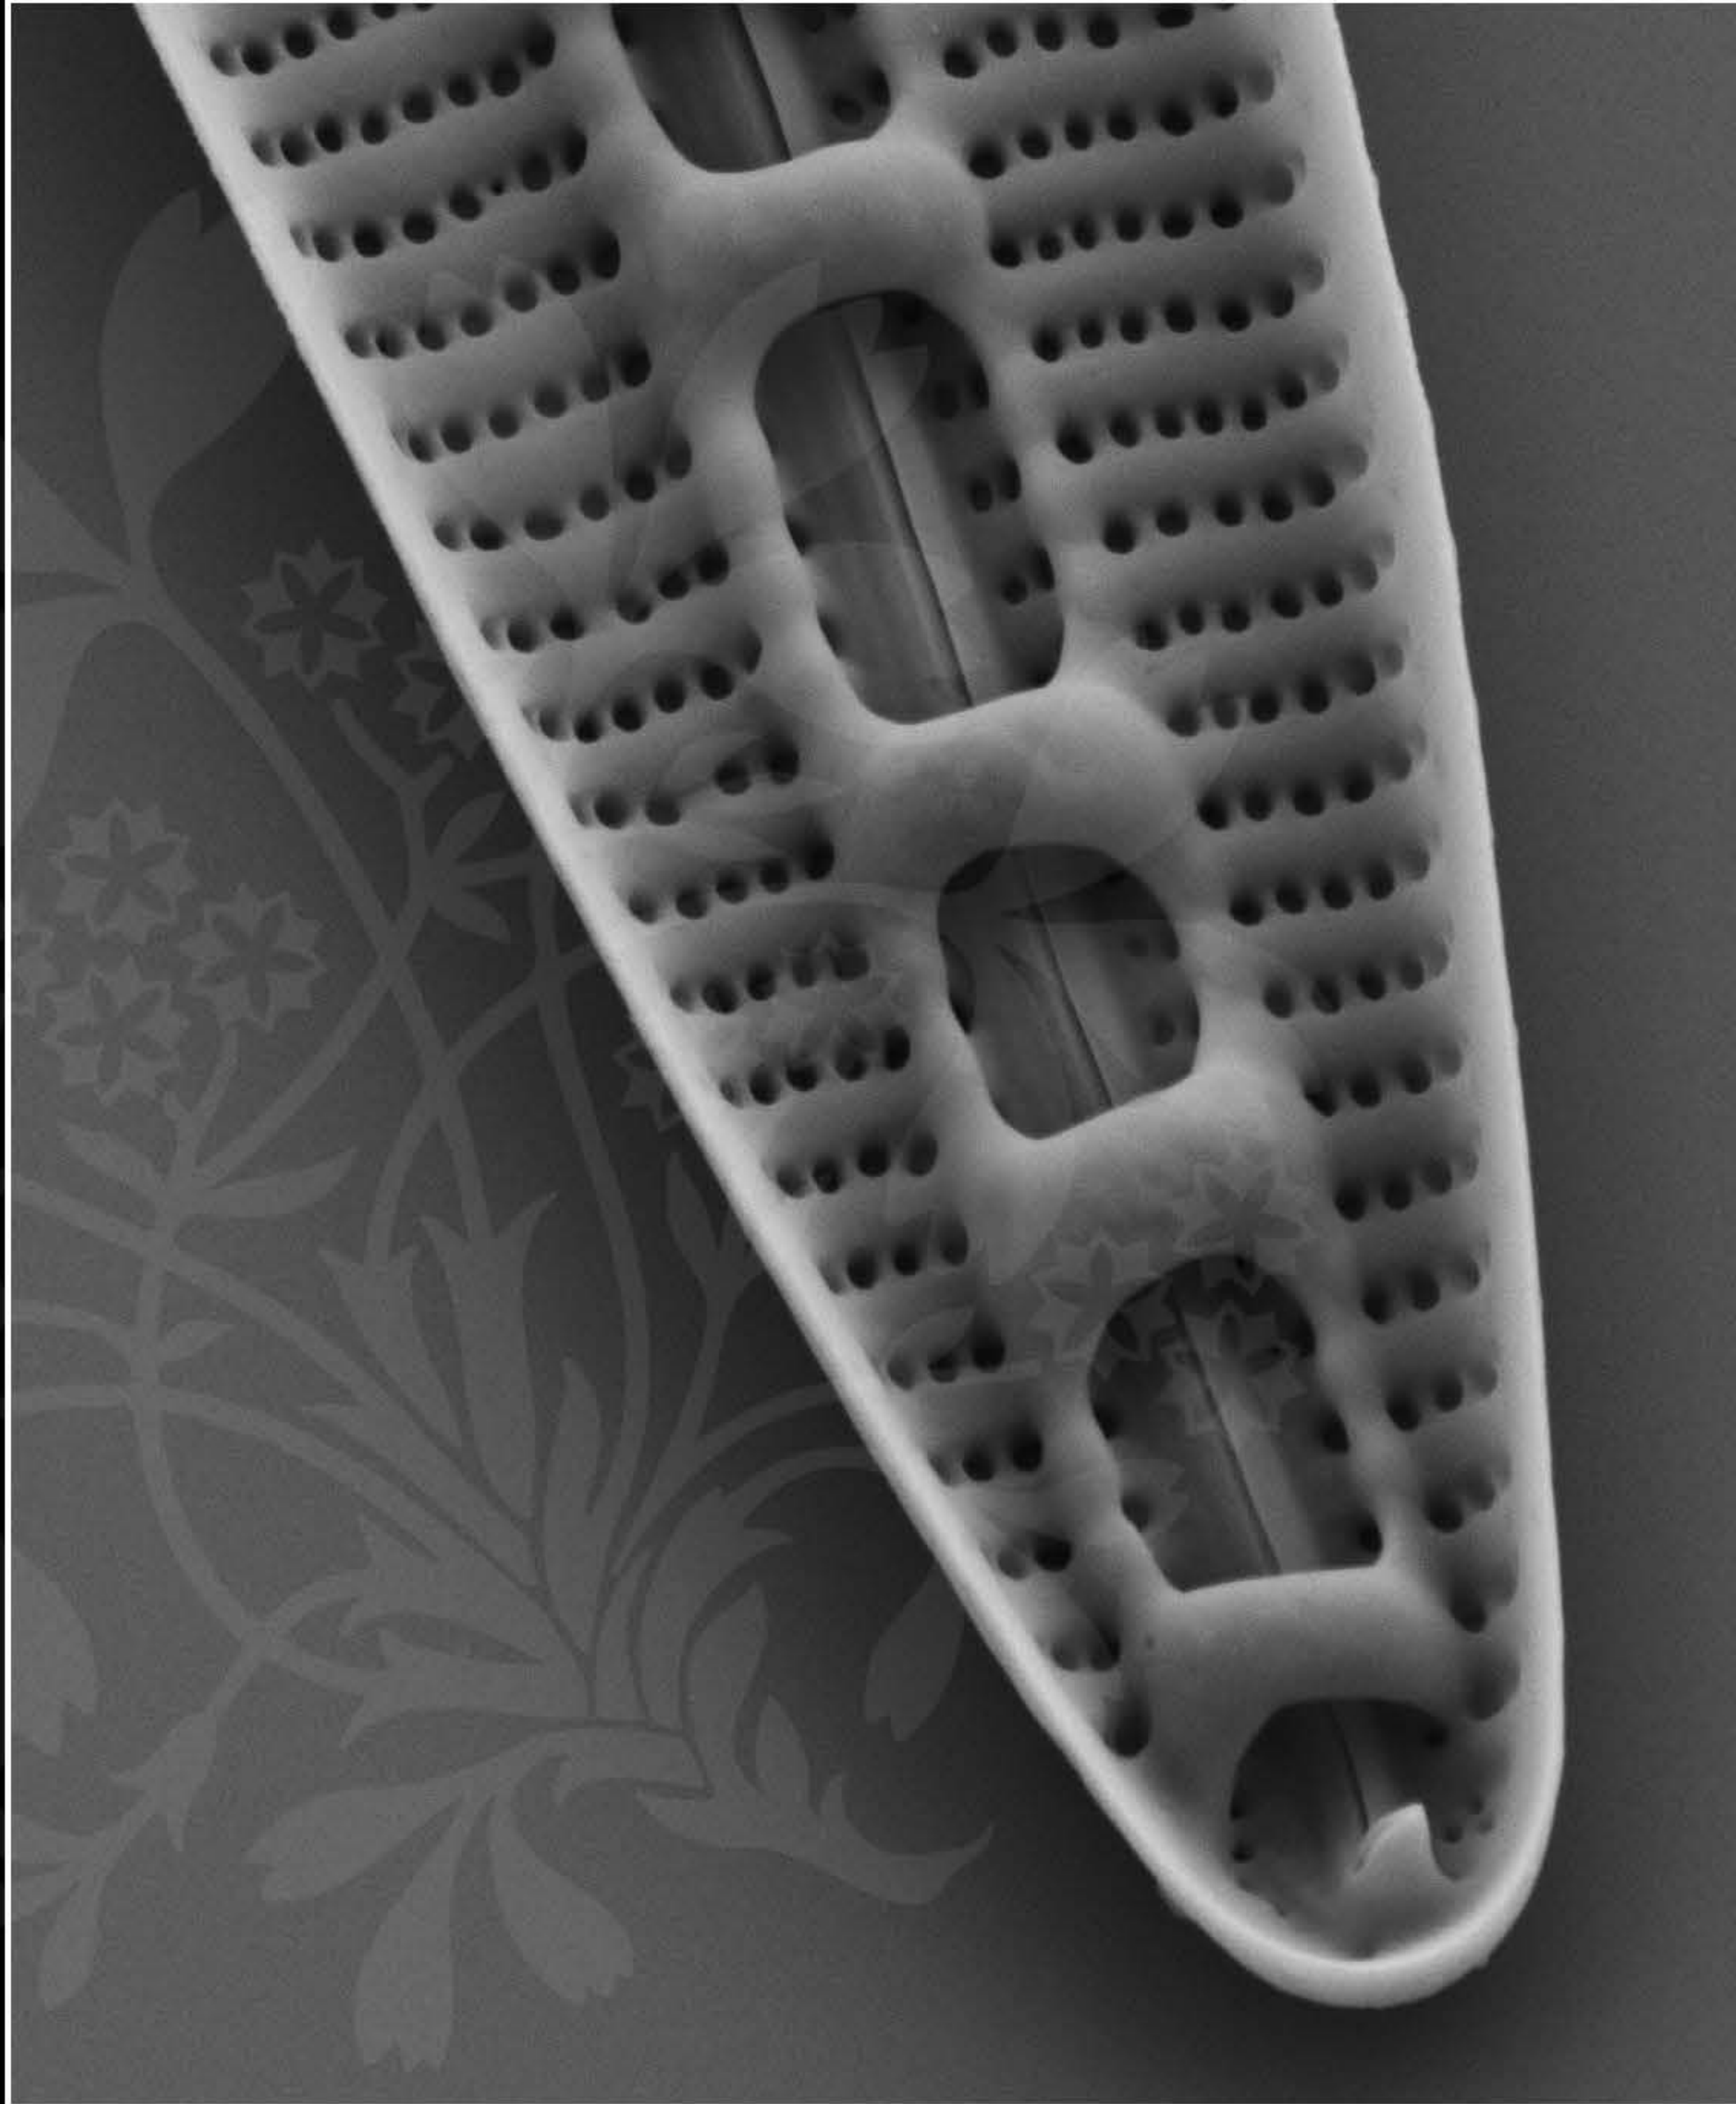

1 μm

Mag = 20.00 K X


EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_18.tif



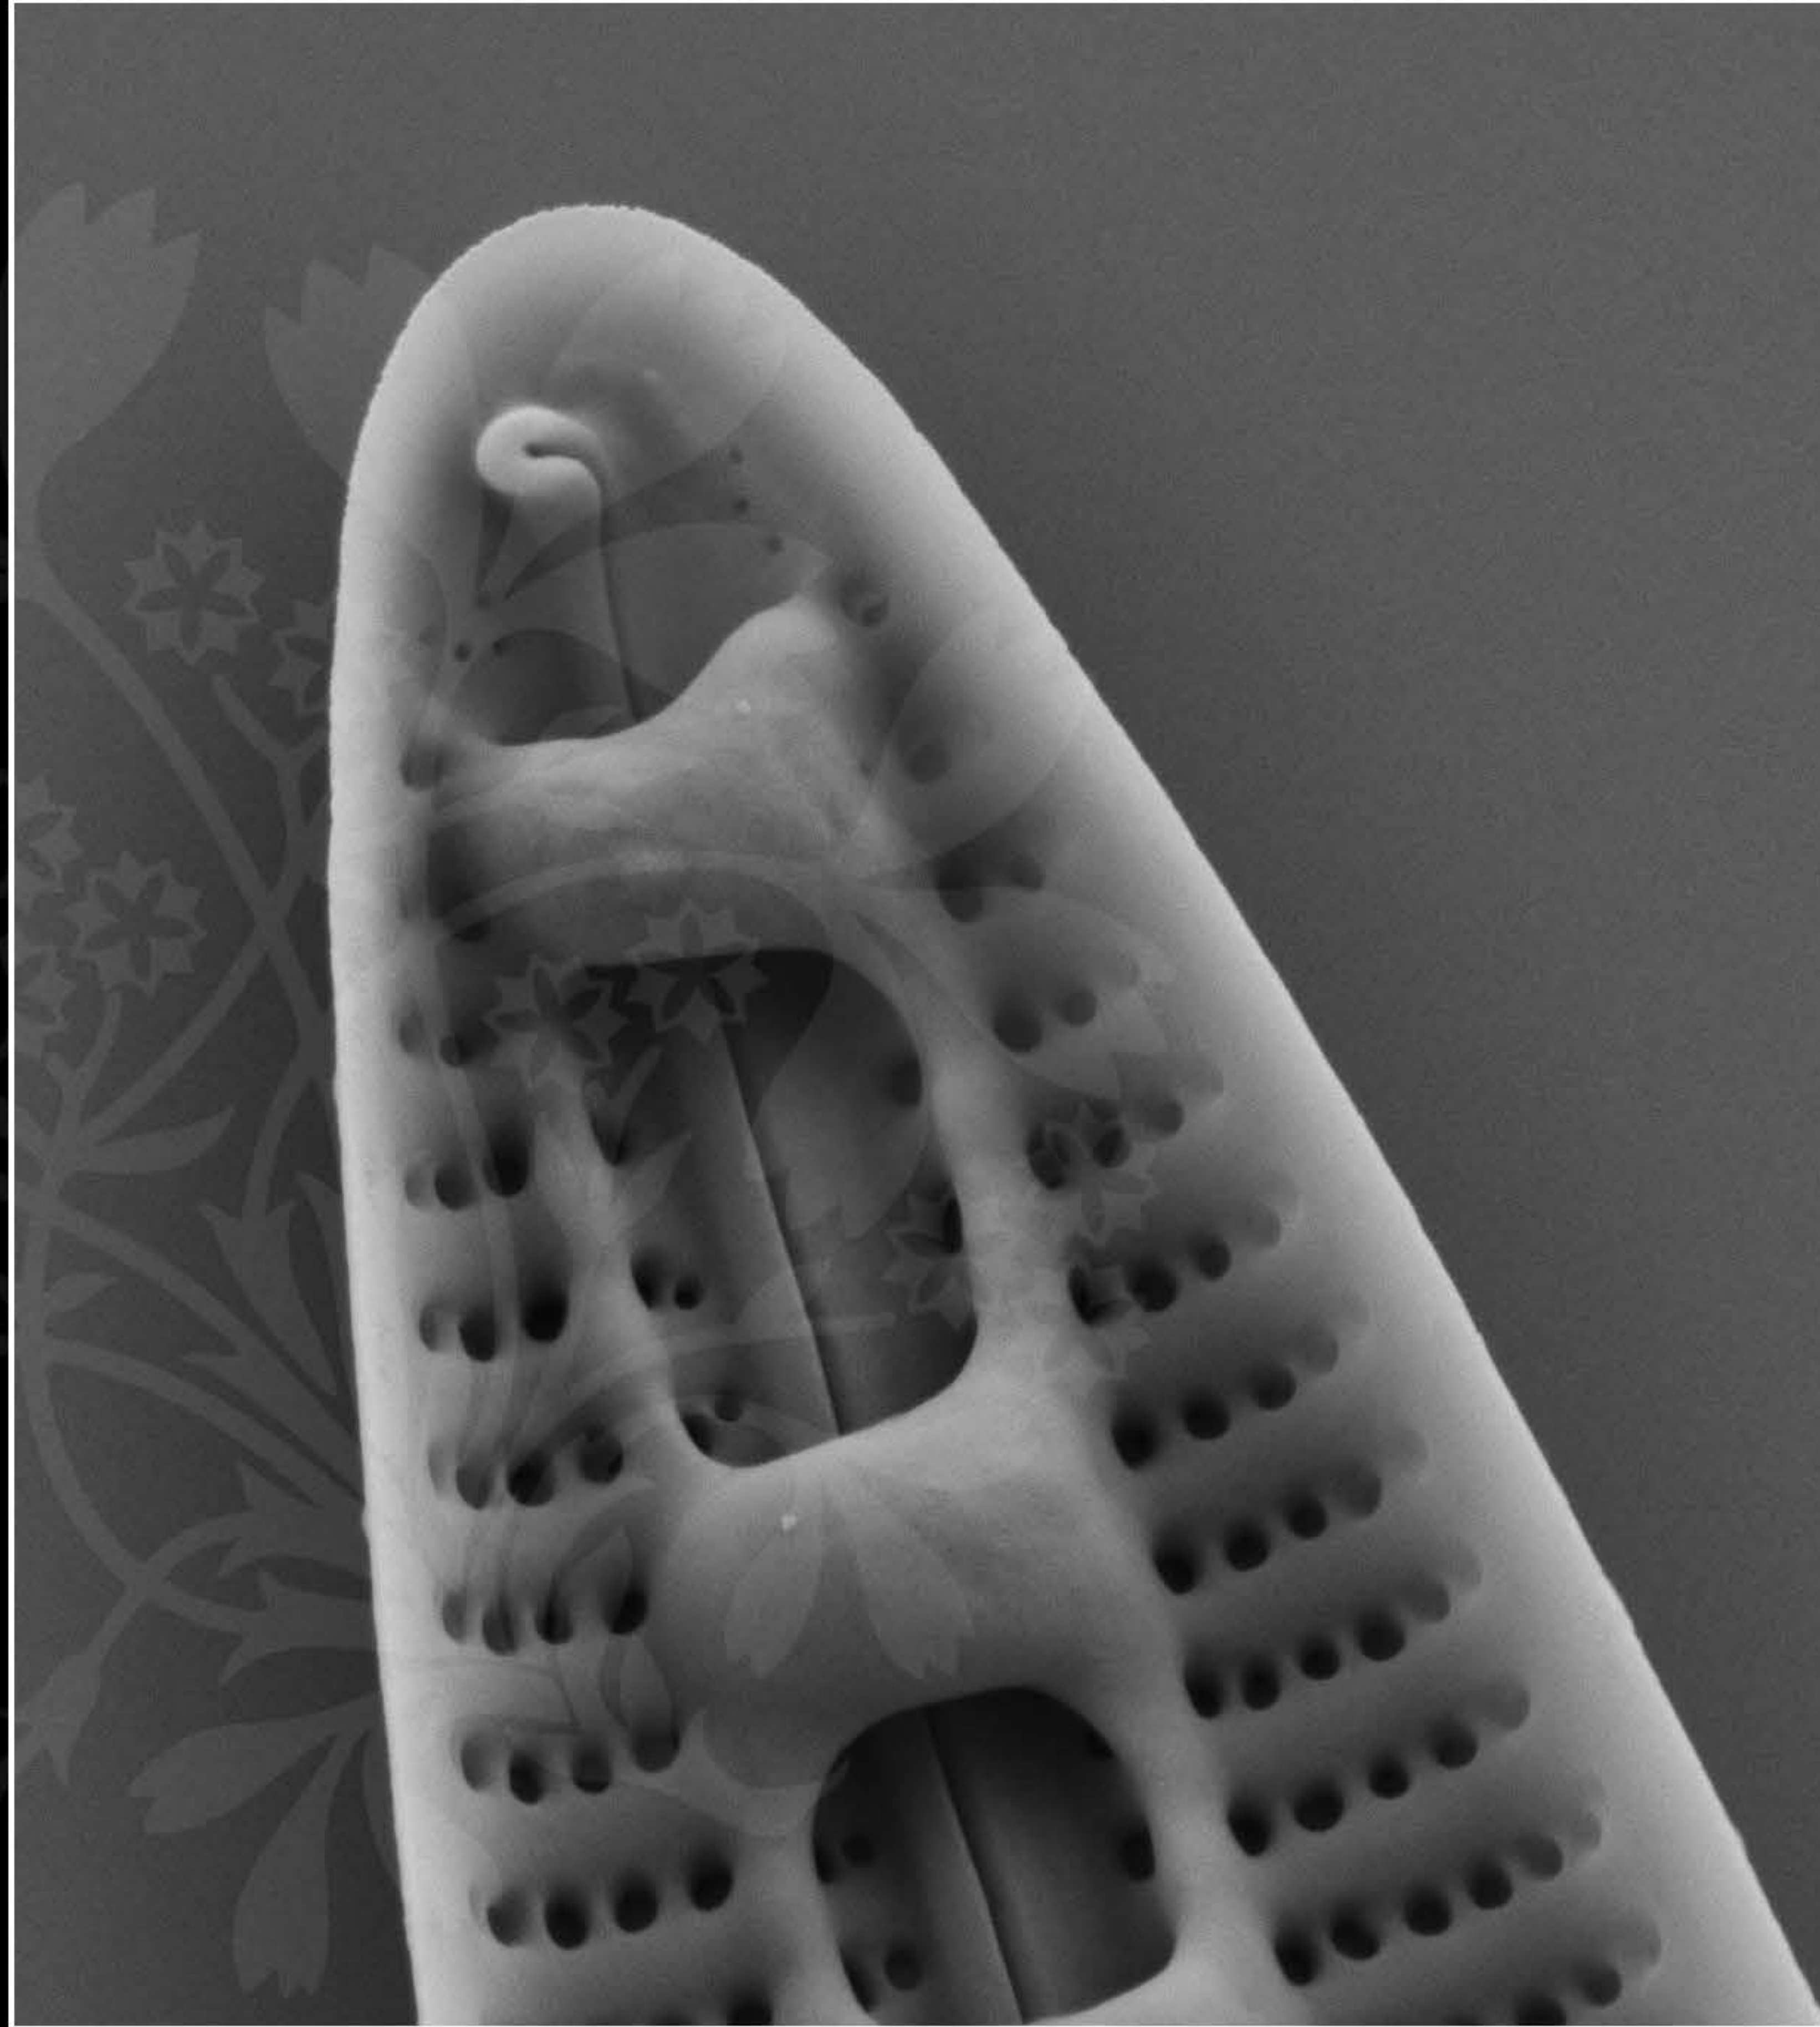

200 nm
└─┘

Mag = 30.00 K X

EHT = 4.50 kV

Signal A = SE2 Date :3 Oct 2017

WD = 4.9 mm

File Name = Bac901CAT_19.tif

