

1 μ m

Mag = 10.00 K X


EHT = 5.00 kV

Signal A = SE2 Date :15 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_01.tif



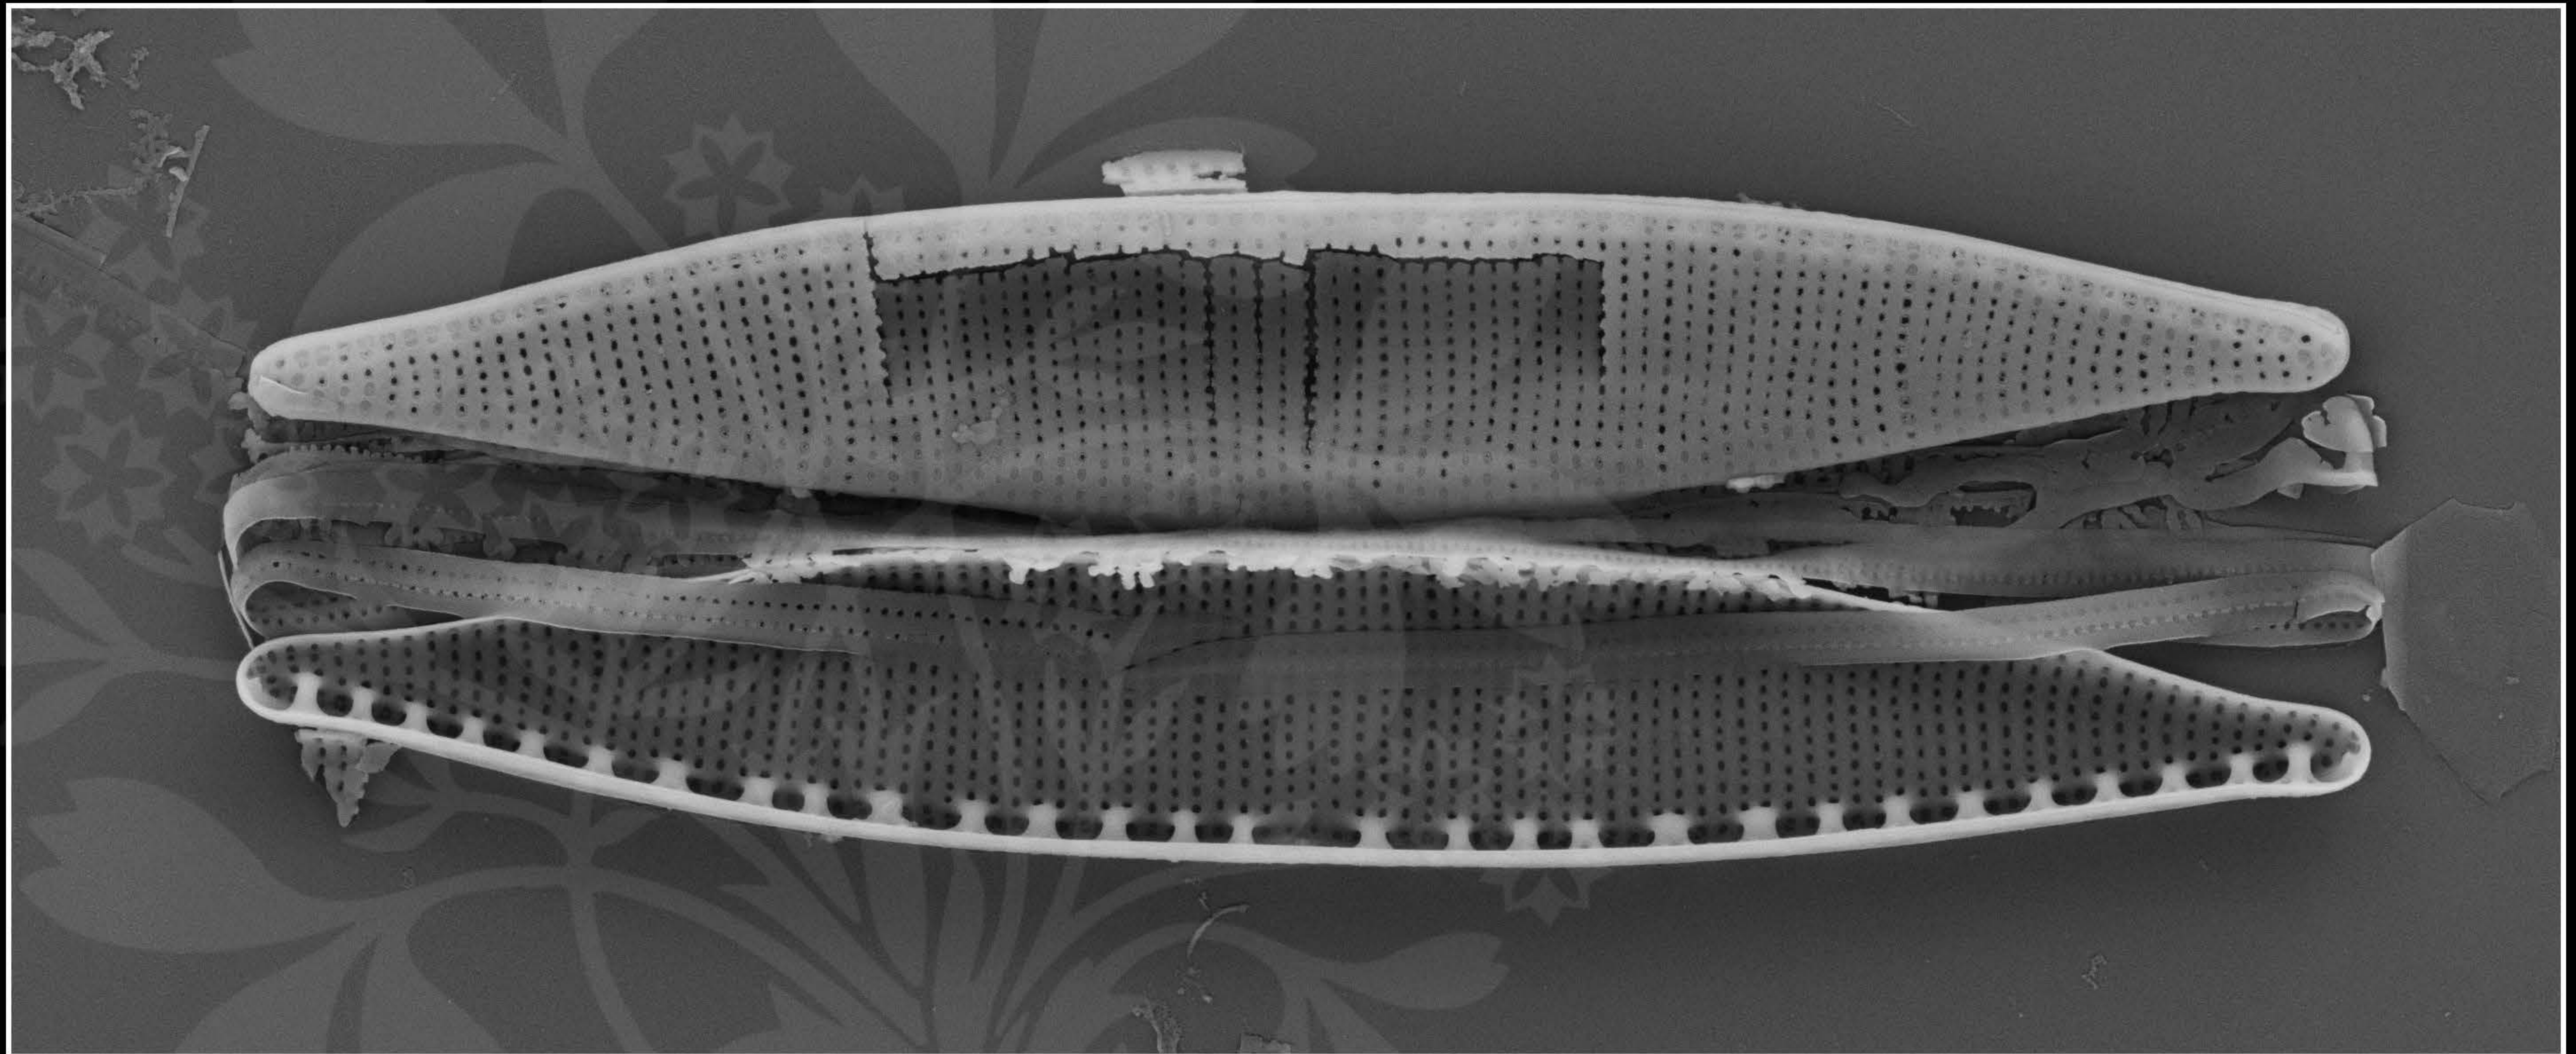

1 μm

Mag = 10.00 K X

EHT = 5.00 kV

Signal A = SE2 Date :15 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_02.tif





200 nm
└───┘

Mag = 40.00 K X


EHT = 5.00 kV

Signal A = SE2 Date :16 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_03.tif



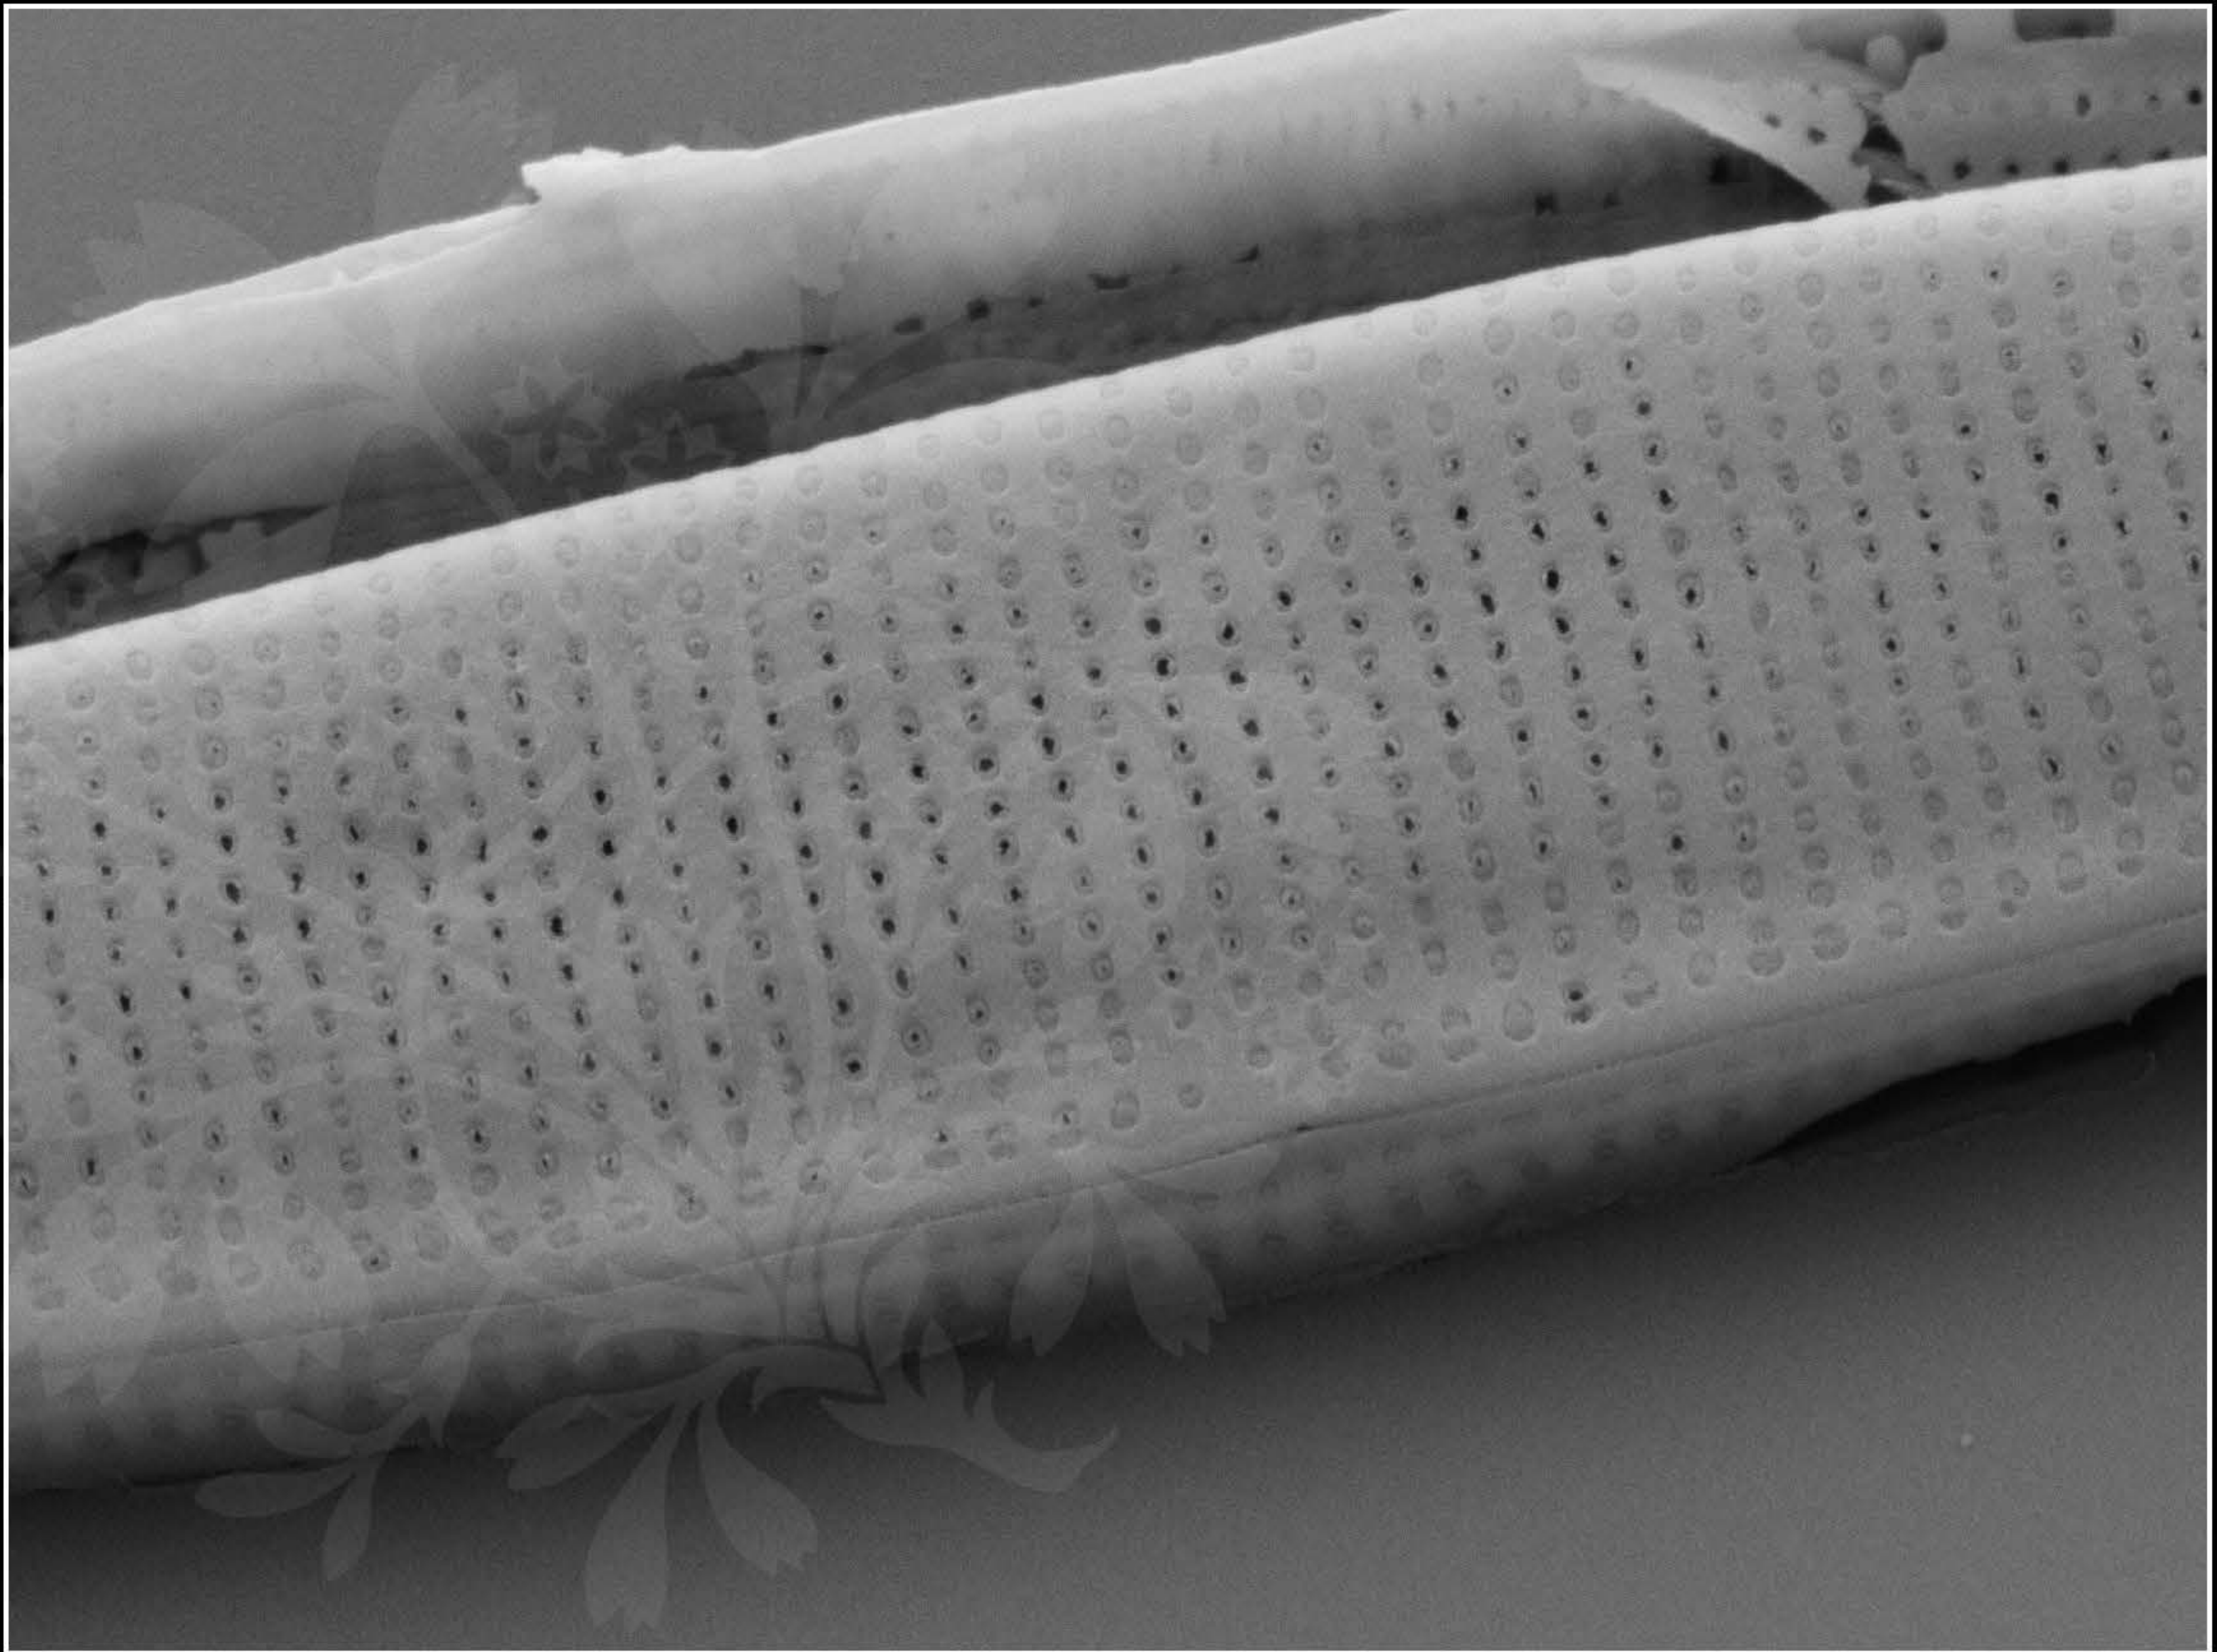

200 nm
└─┘

Mag = 30.00 K X


EHT = 5.00 kV

Signal A = SE2 Date :16 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_04.tif



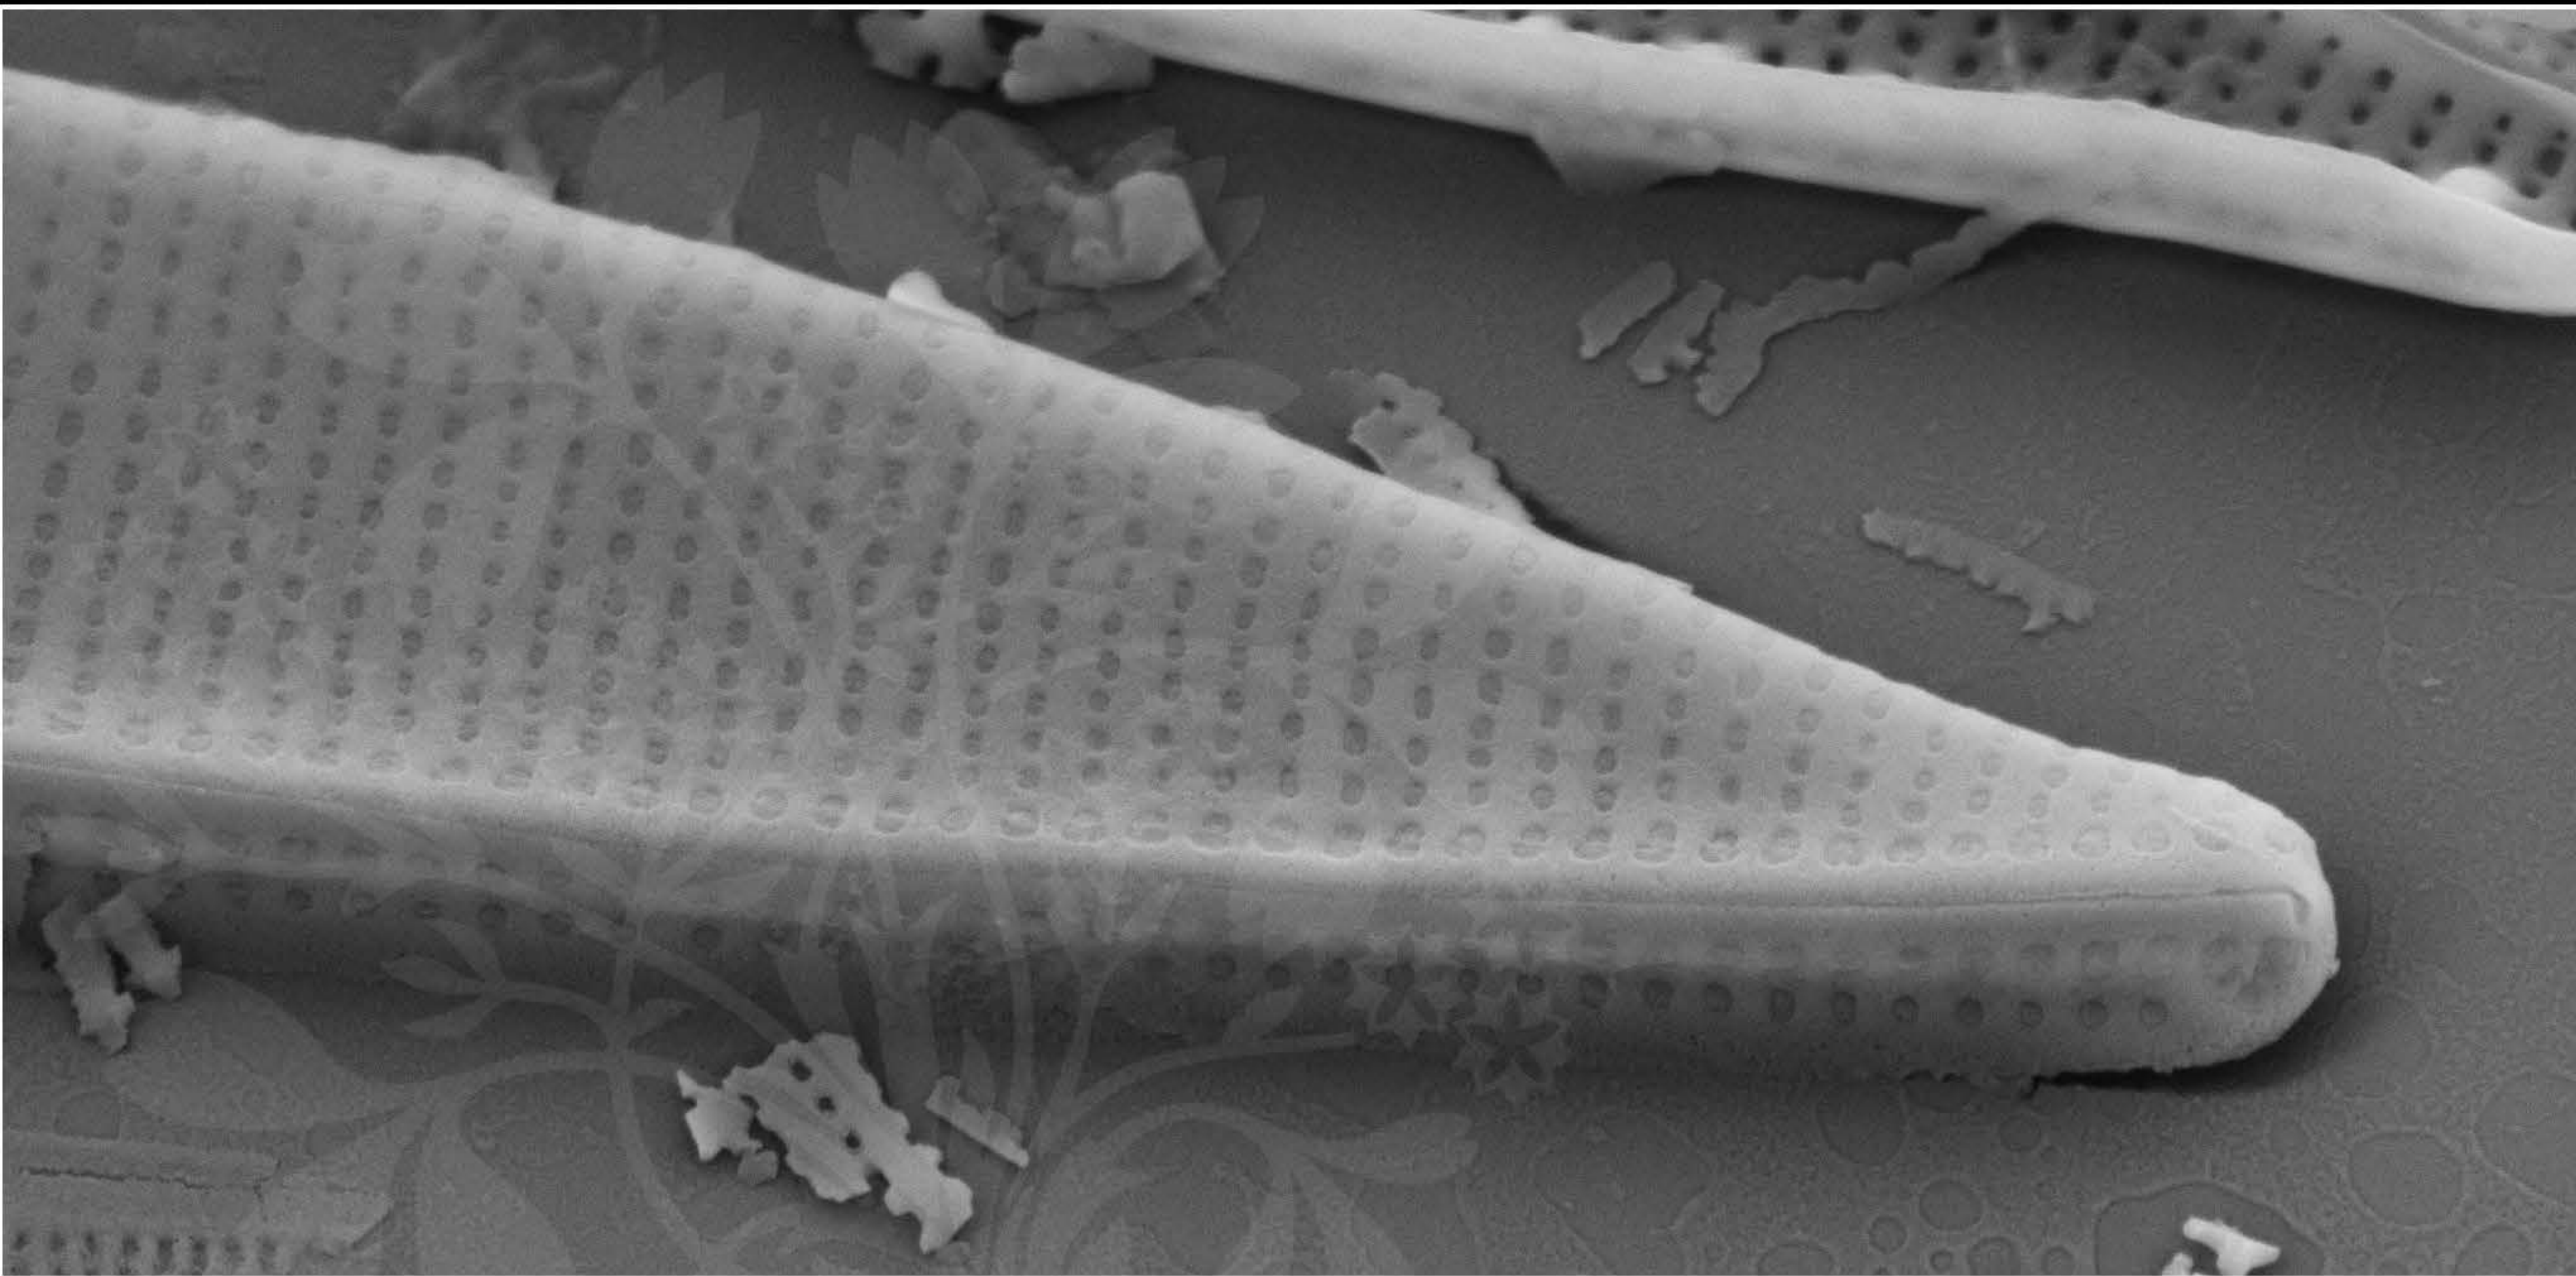

200 nm
└─┘

Mag = 30.00 K X


EHT = 5.00 kV

Signal A = SE2 Date :16 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_05.tif



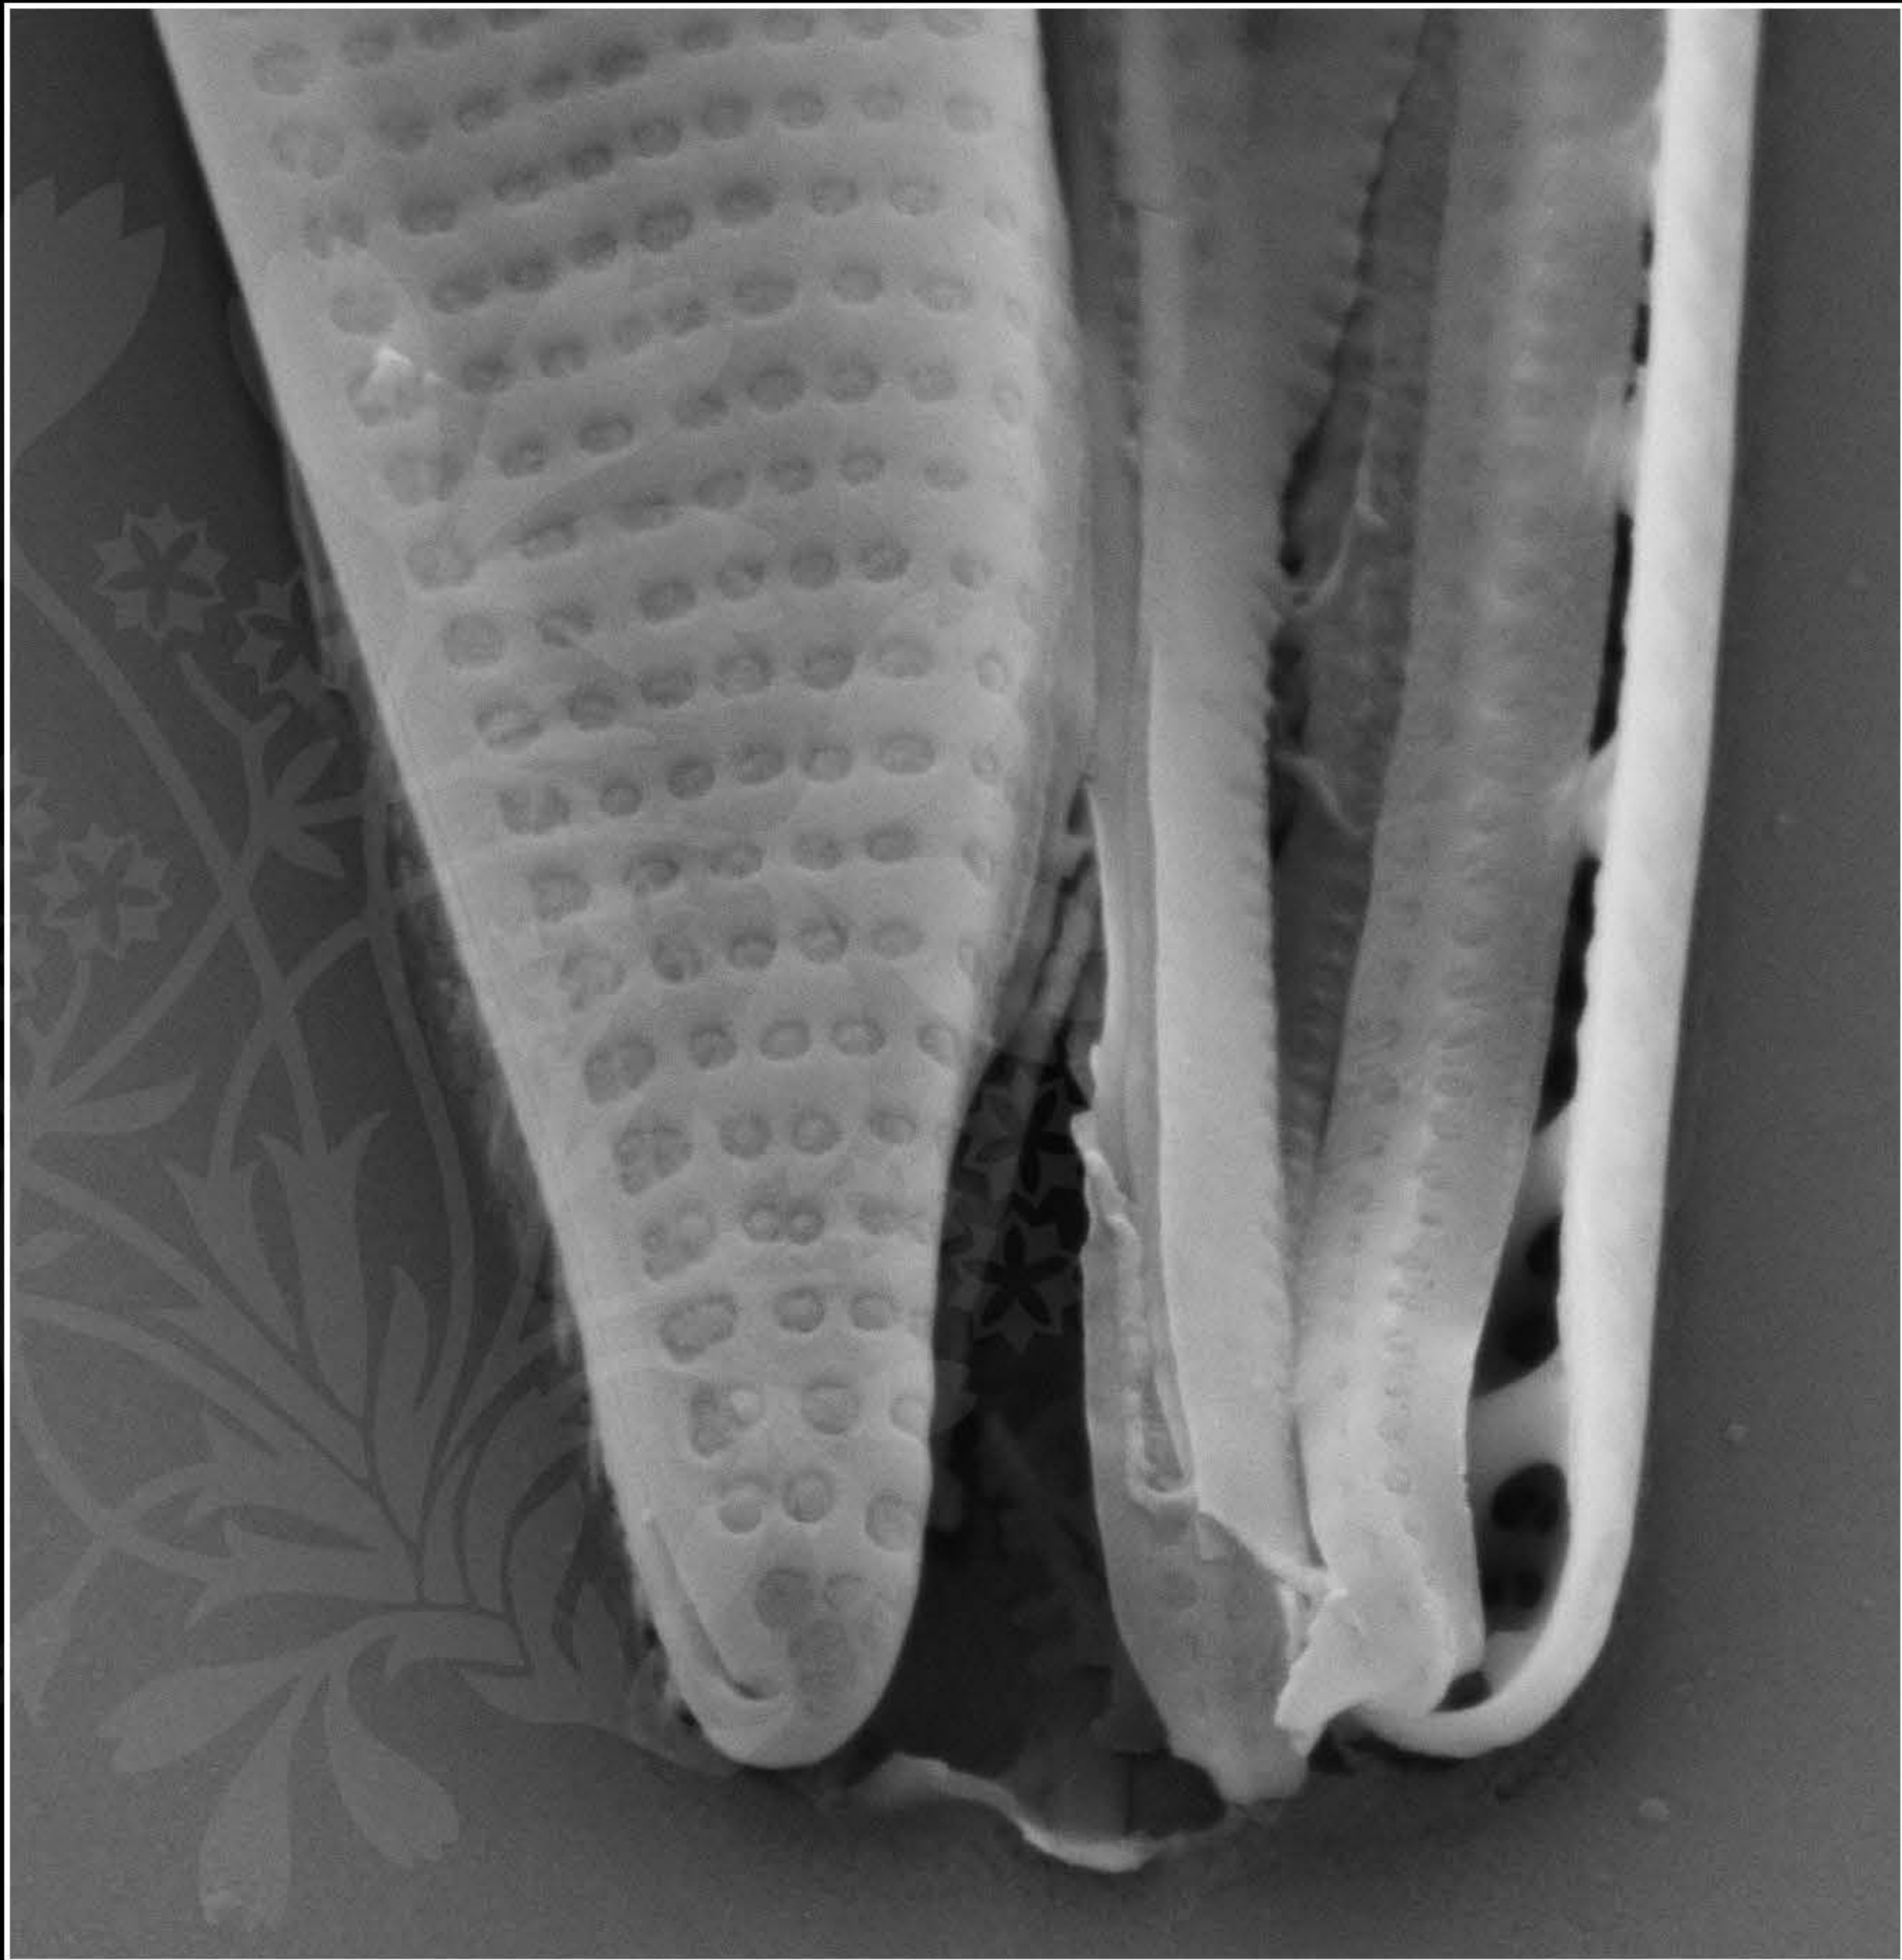

200 nm
└───┘

Mag = 40.00 K X


EHT = 5.00 kV

Signal A = SE2 Date :16 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_06.tif



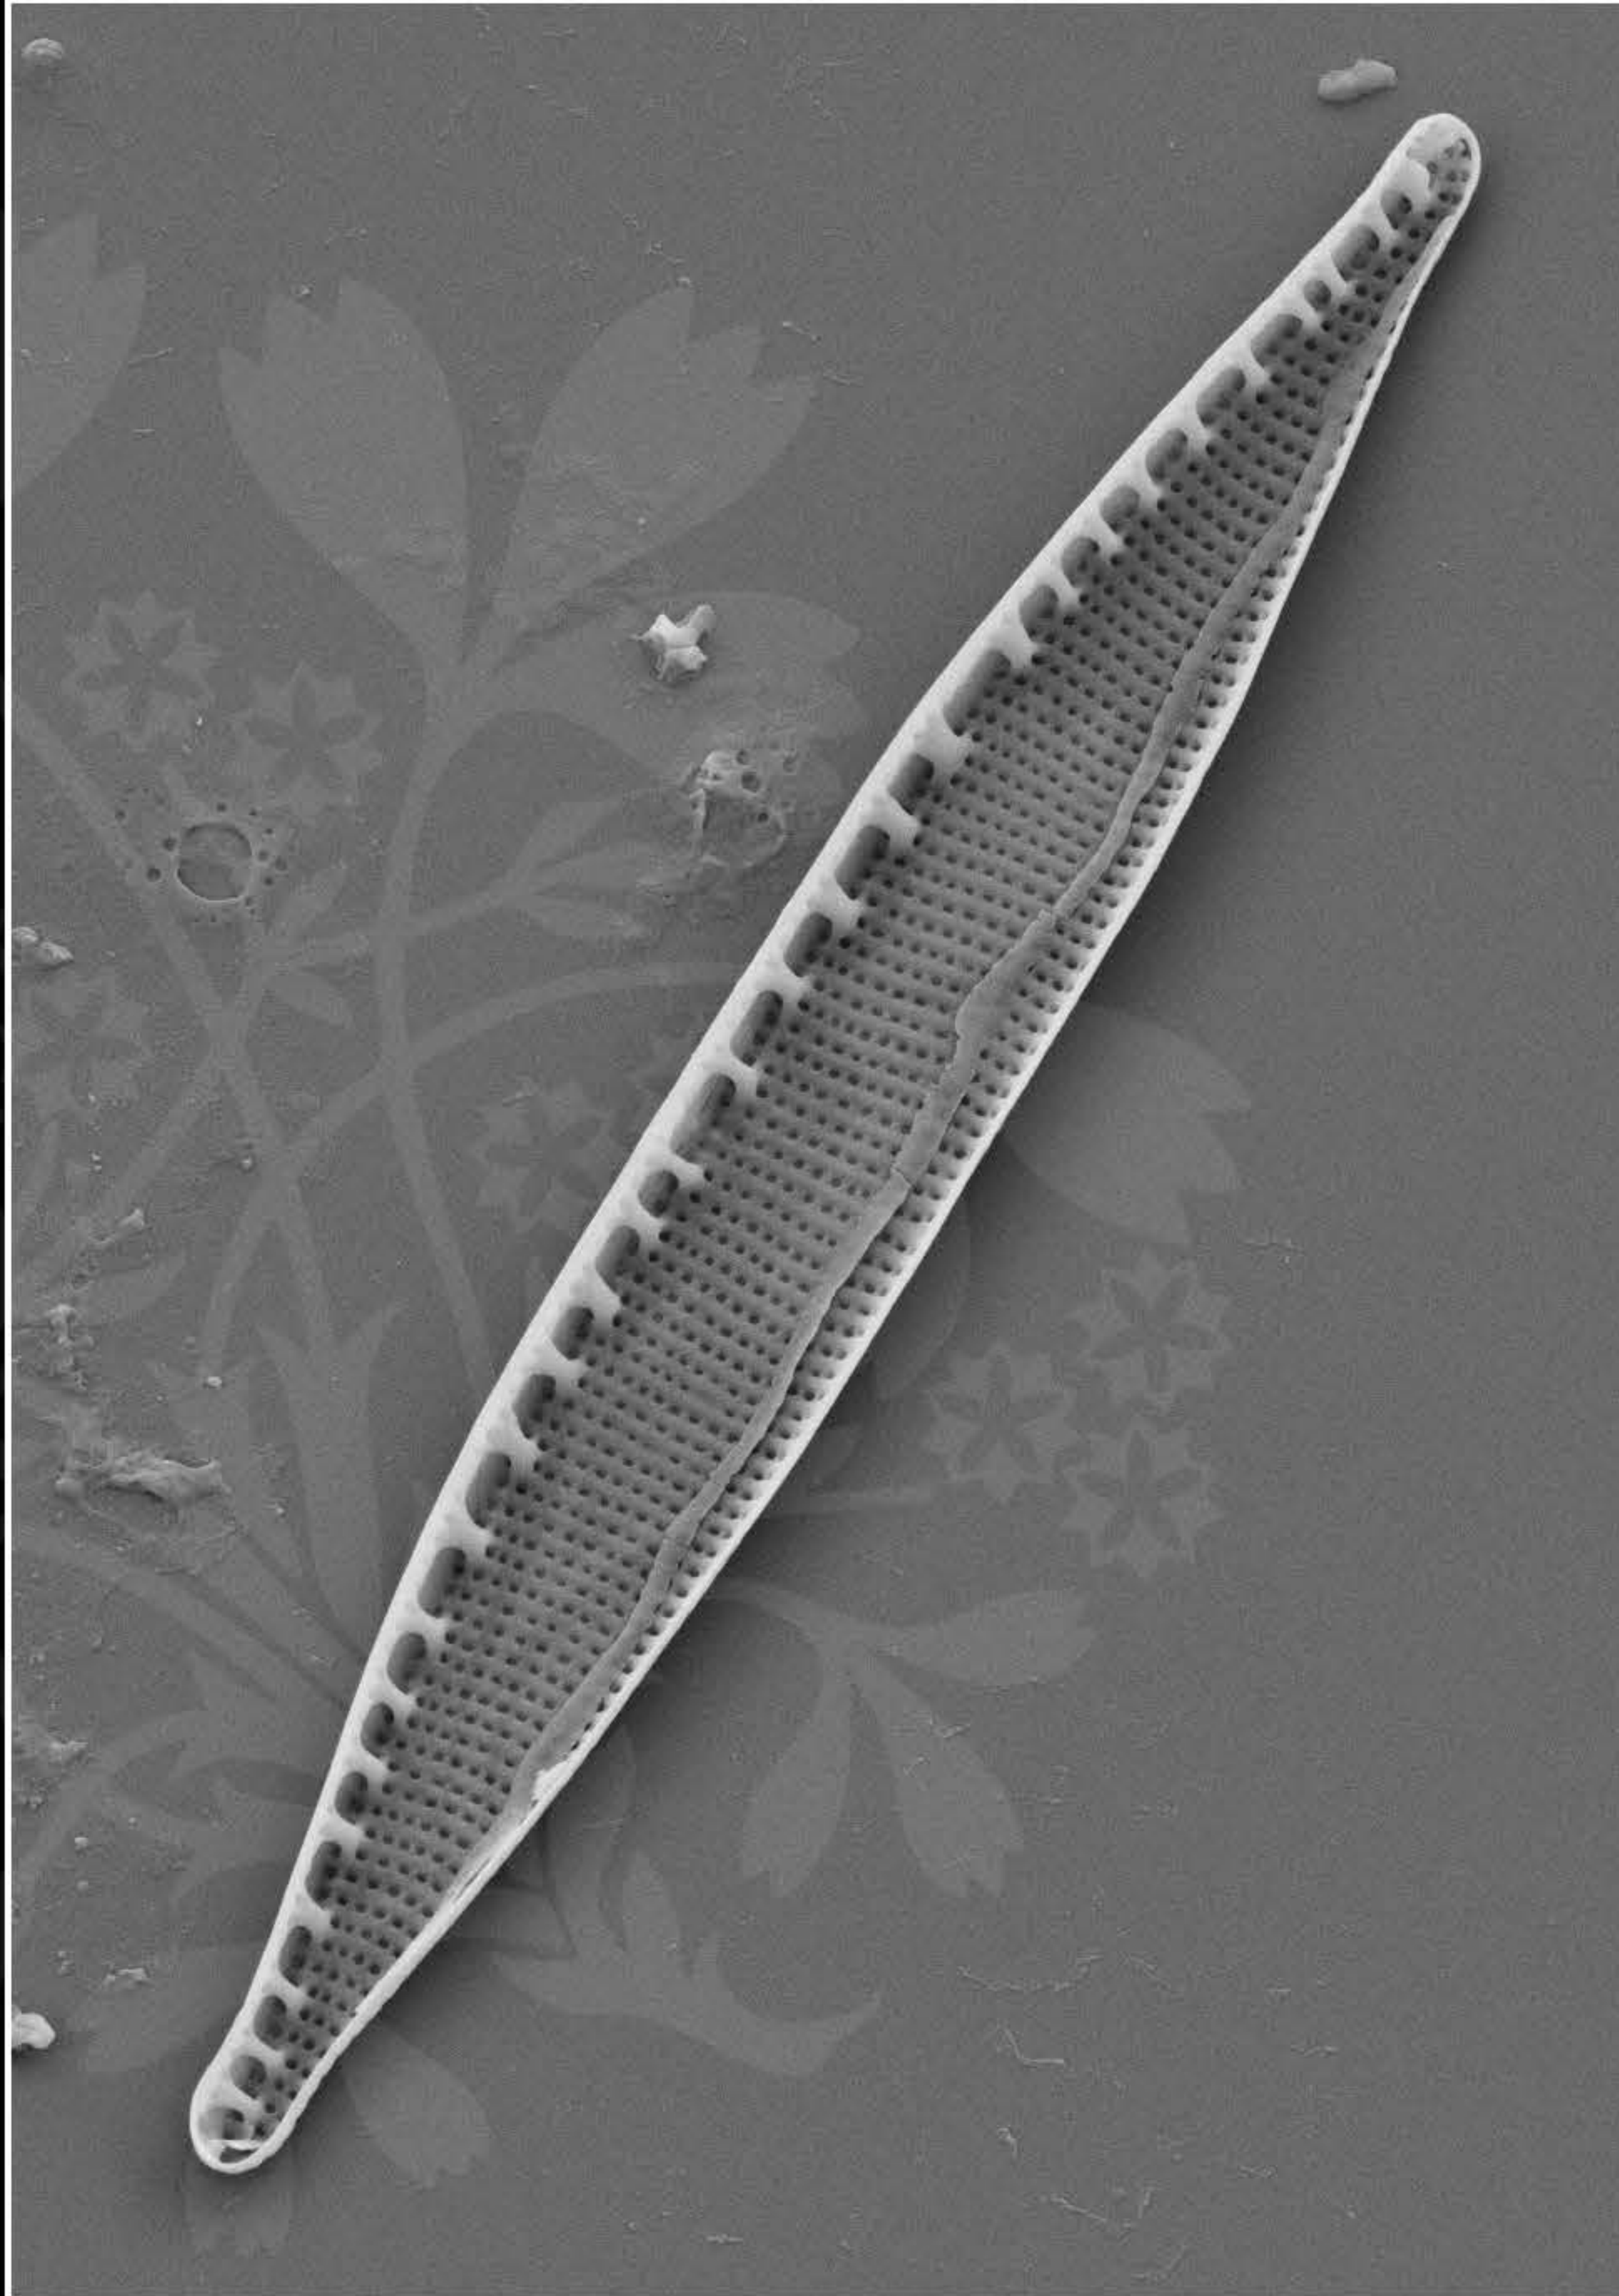

1 μm

Mag = 9.00 K X


EHT = 5.00 kV

Signal A = SE2 Date :16 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_07.tif



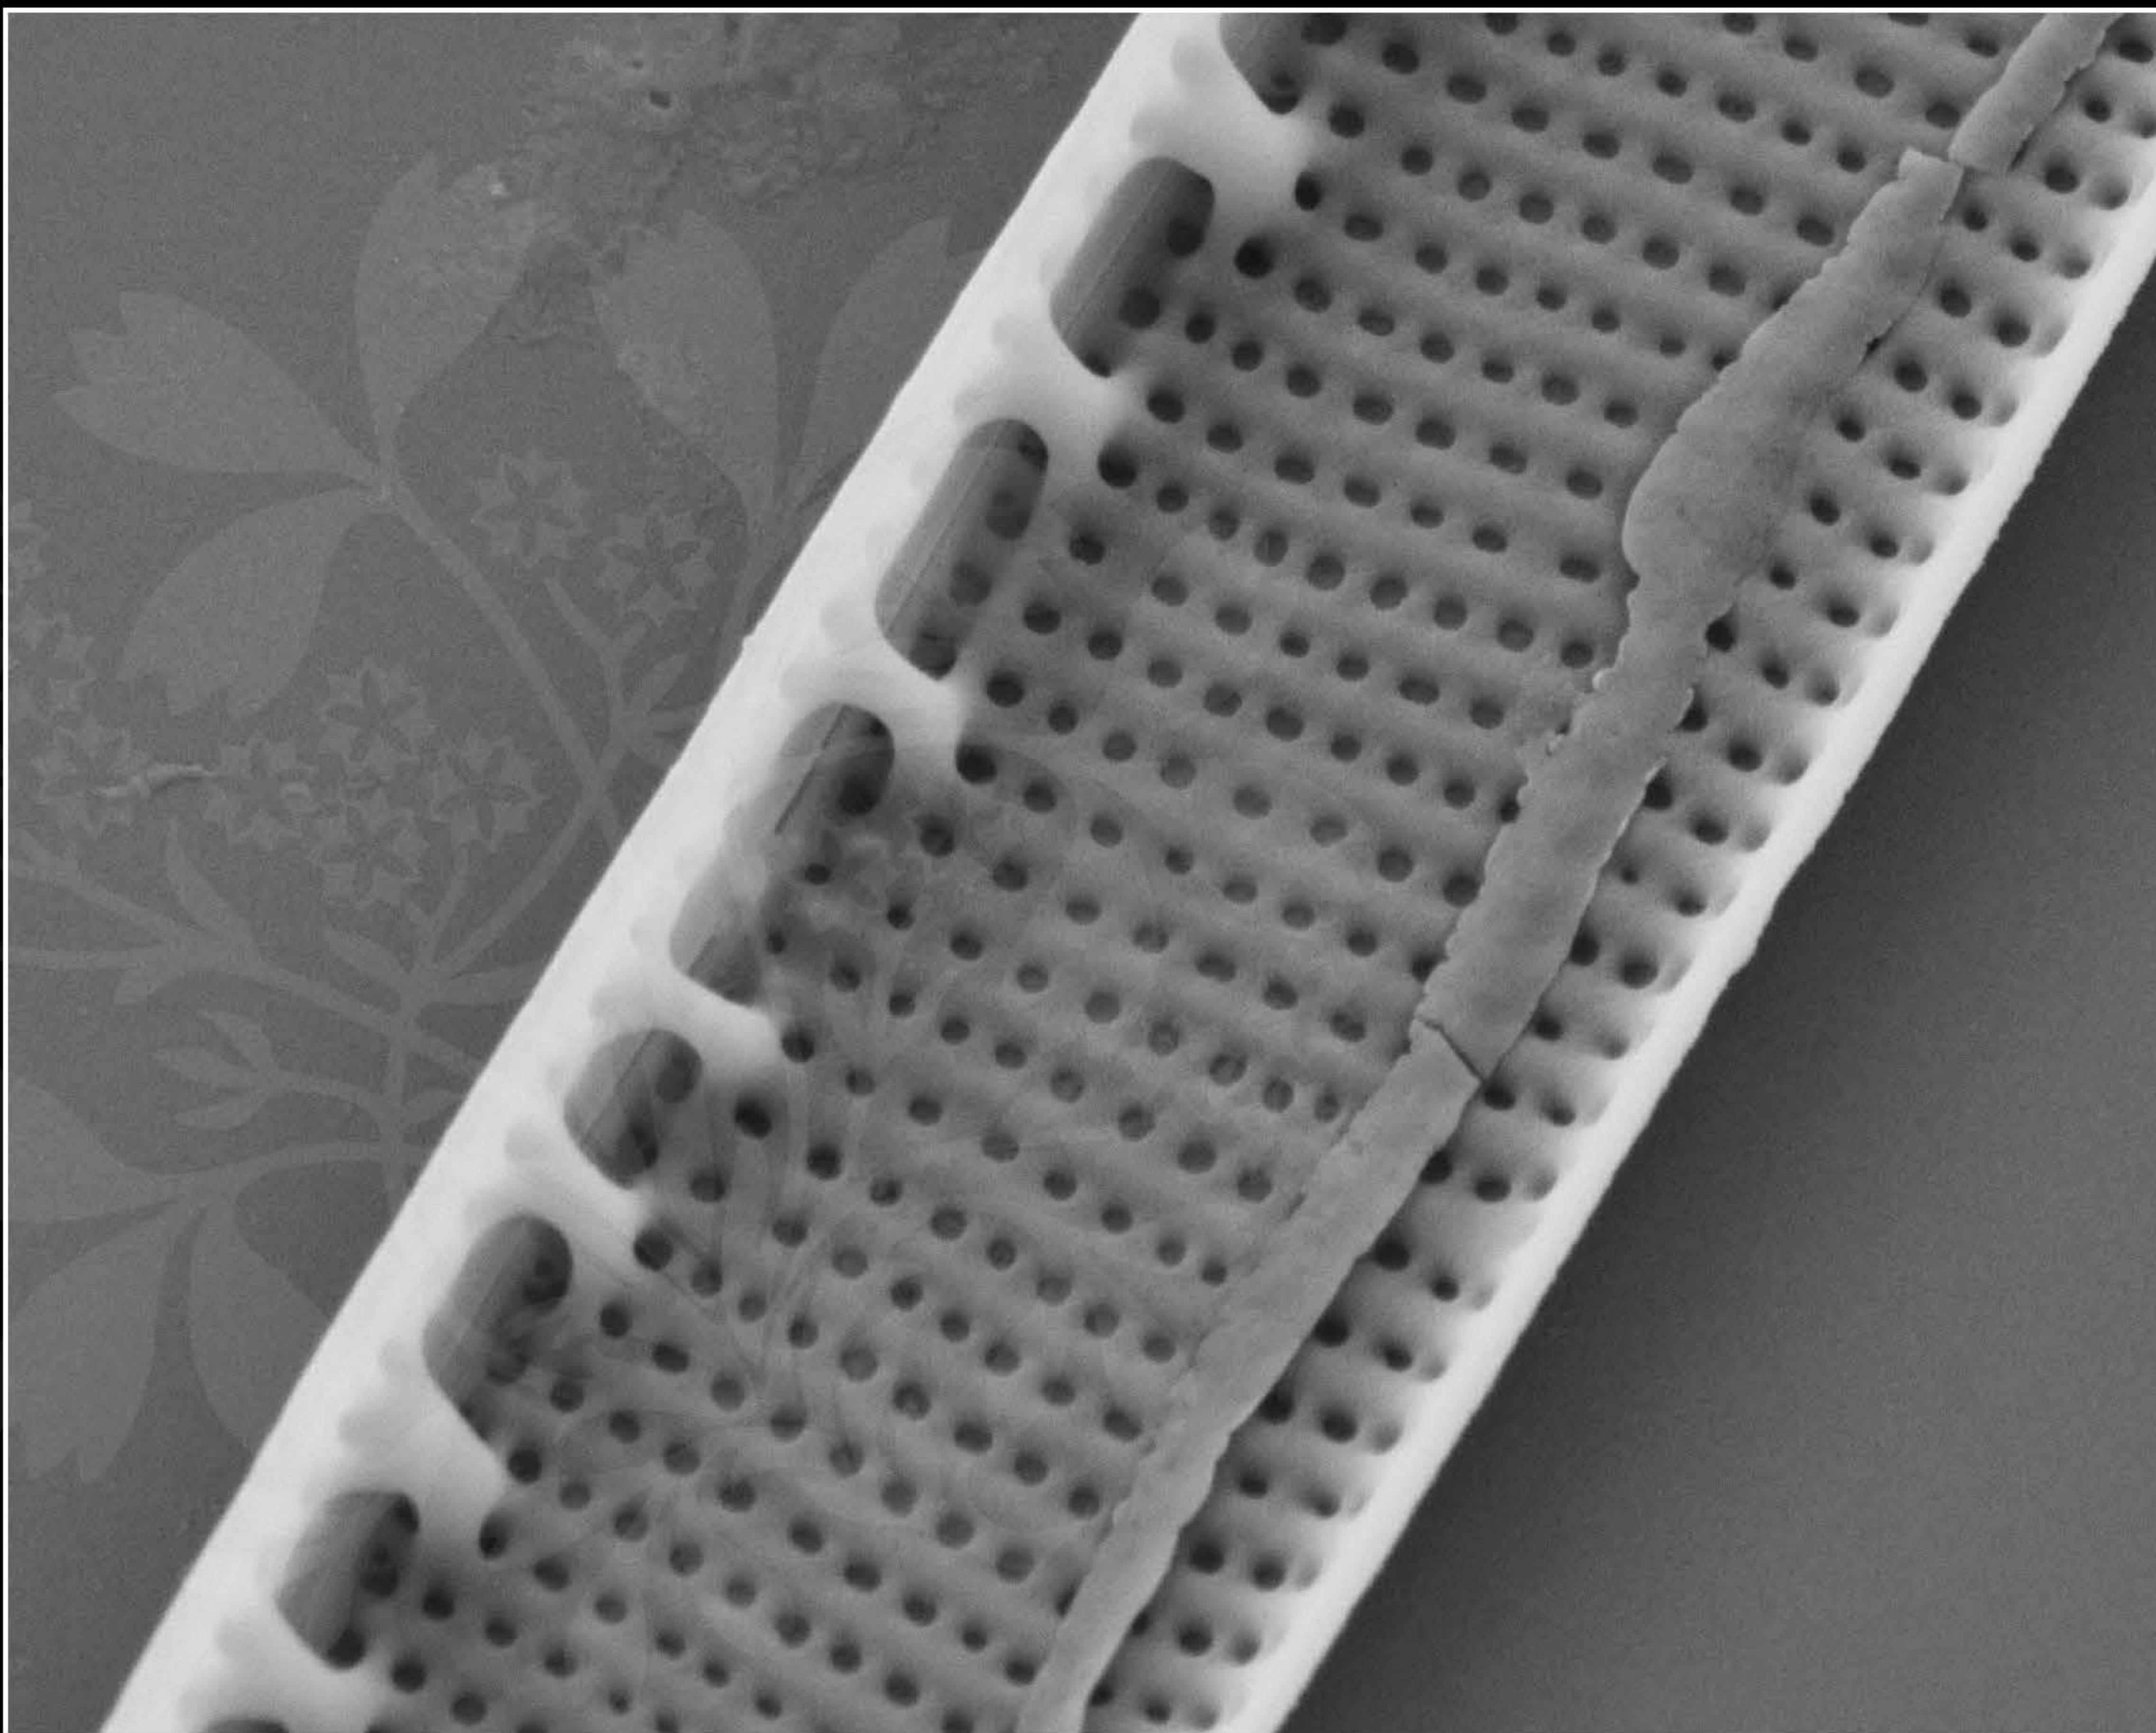

200 nm
└───┘

Mag = 40.00 K X


EHT = 5.00 kV

Signal A = SE2 Date :16 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_08.tif



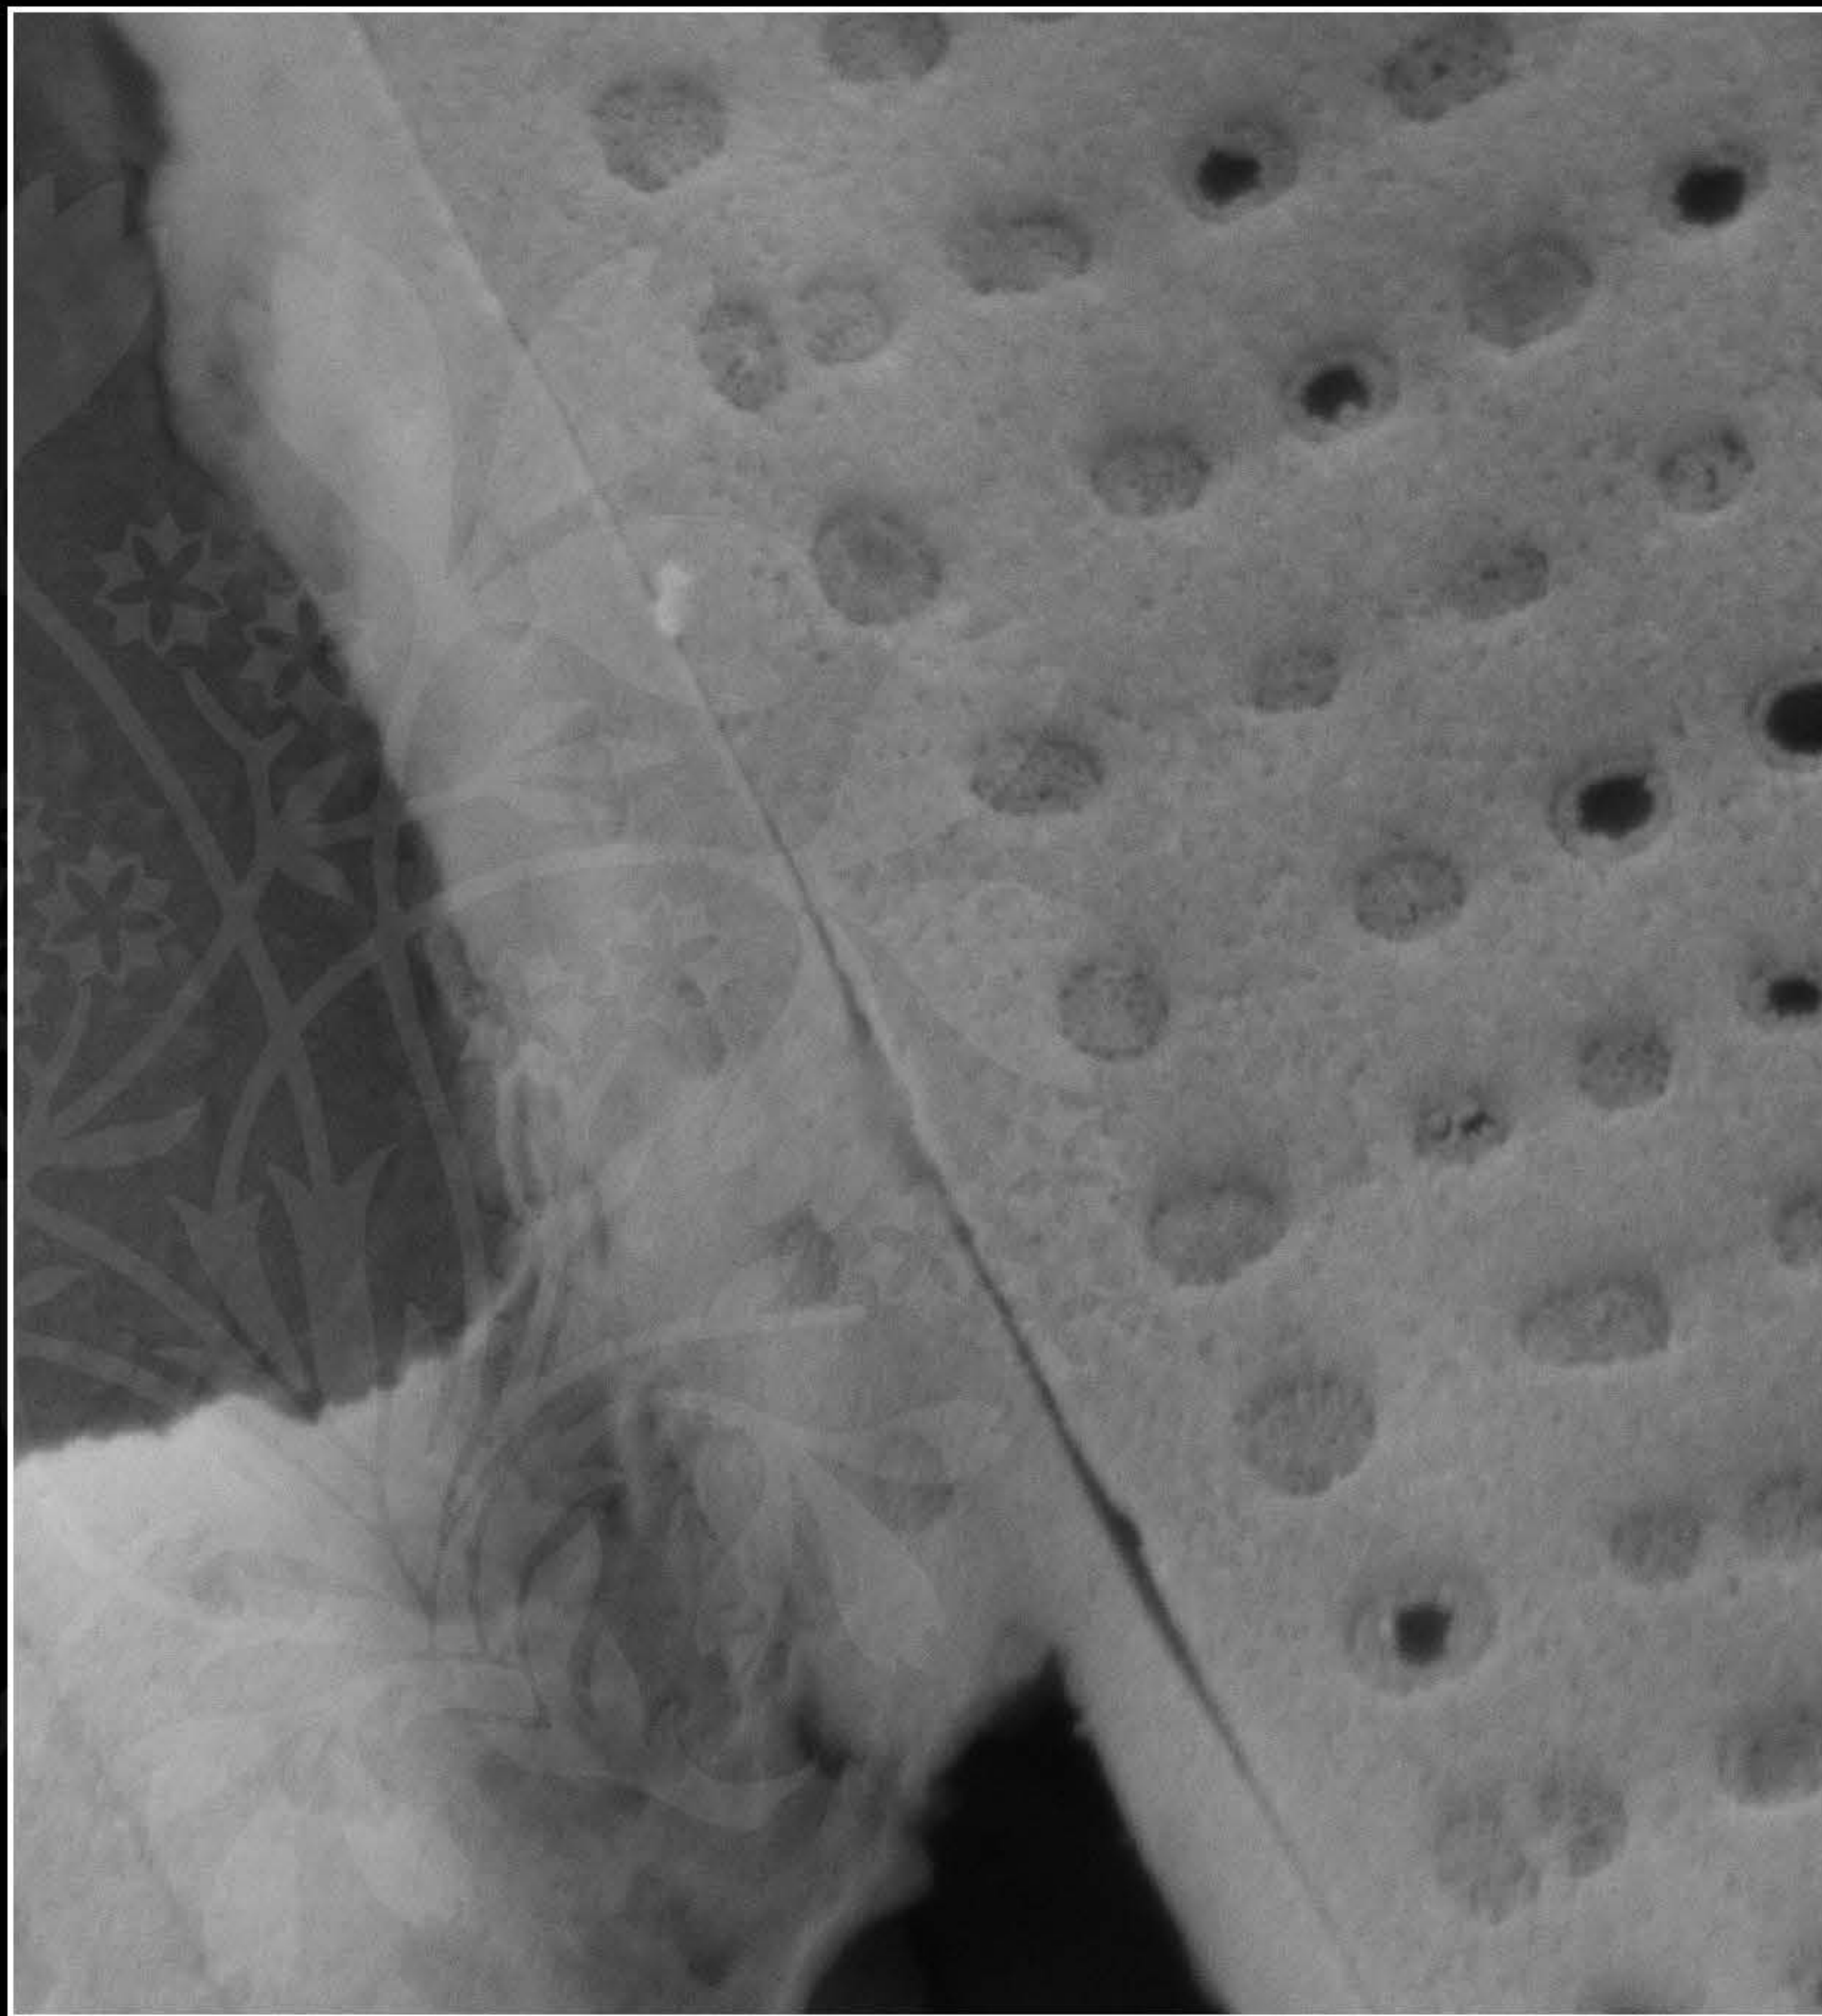

200 nm

Mag = 100.00 K X


EHT = 5.00 kV

Signal A = SE2 Date :16 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_09.tif



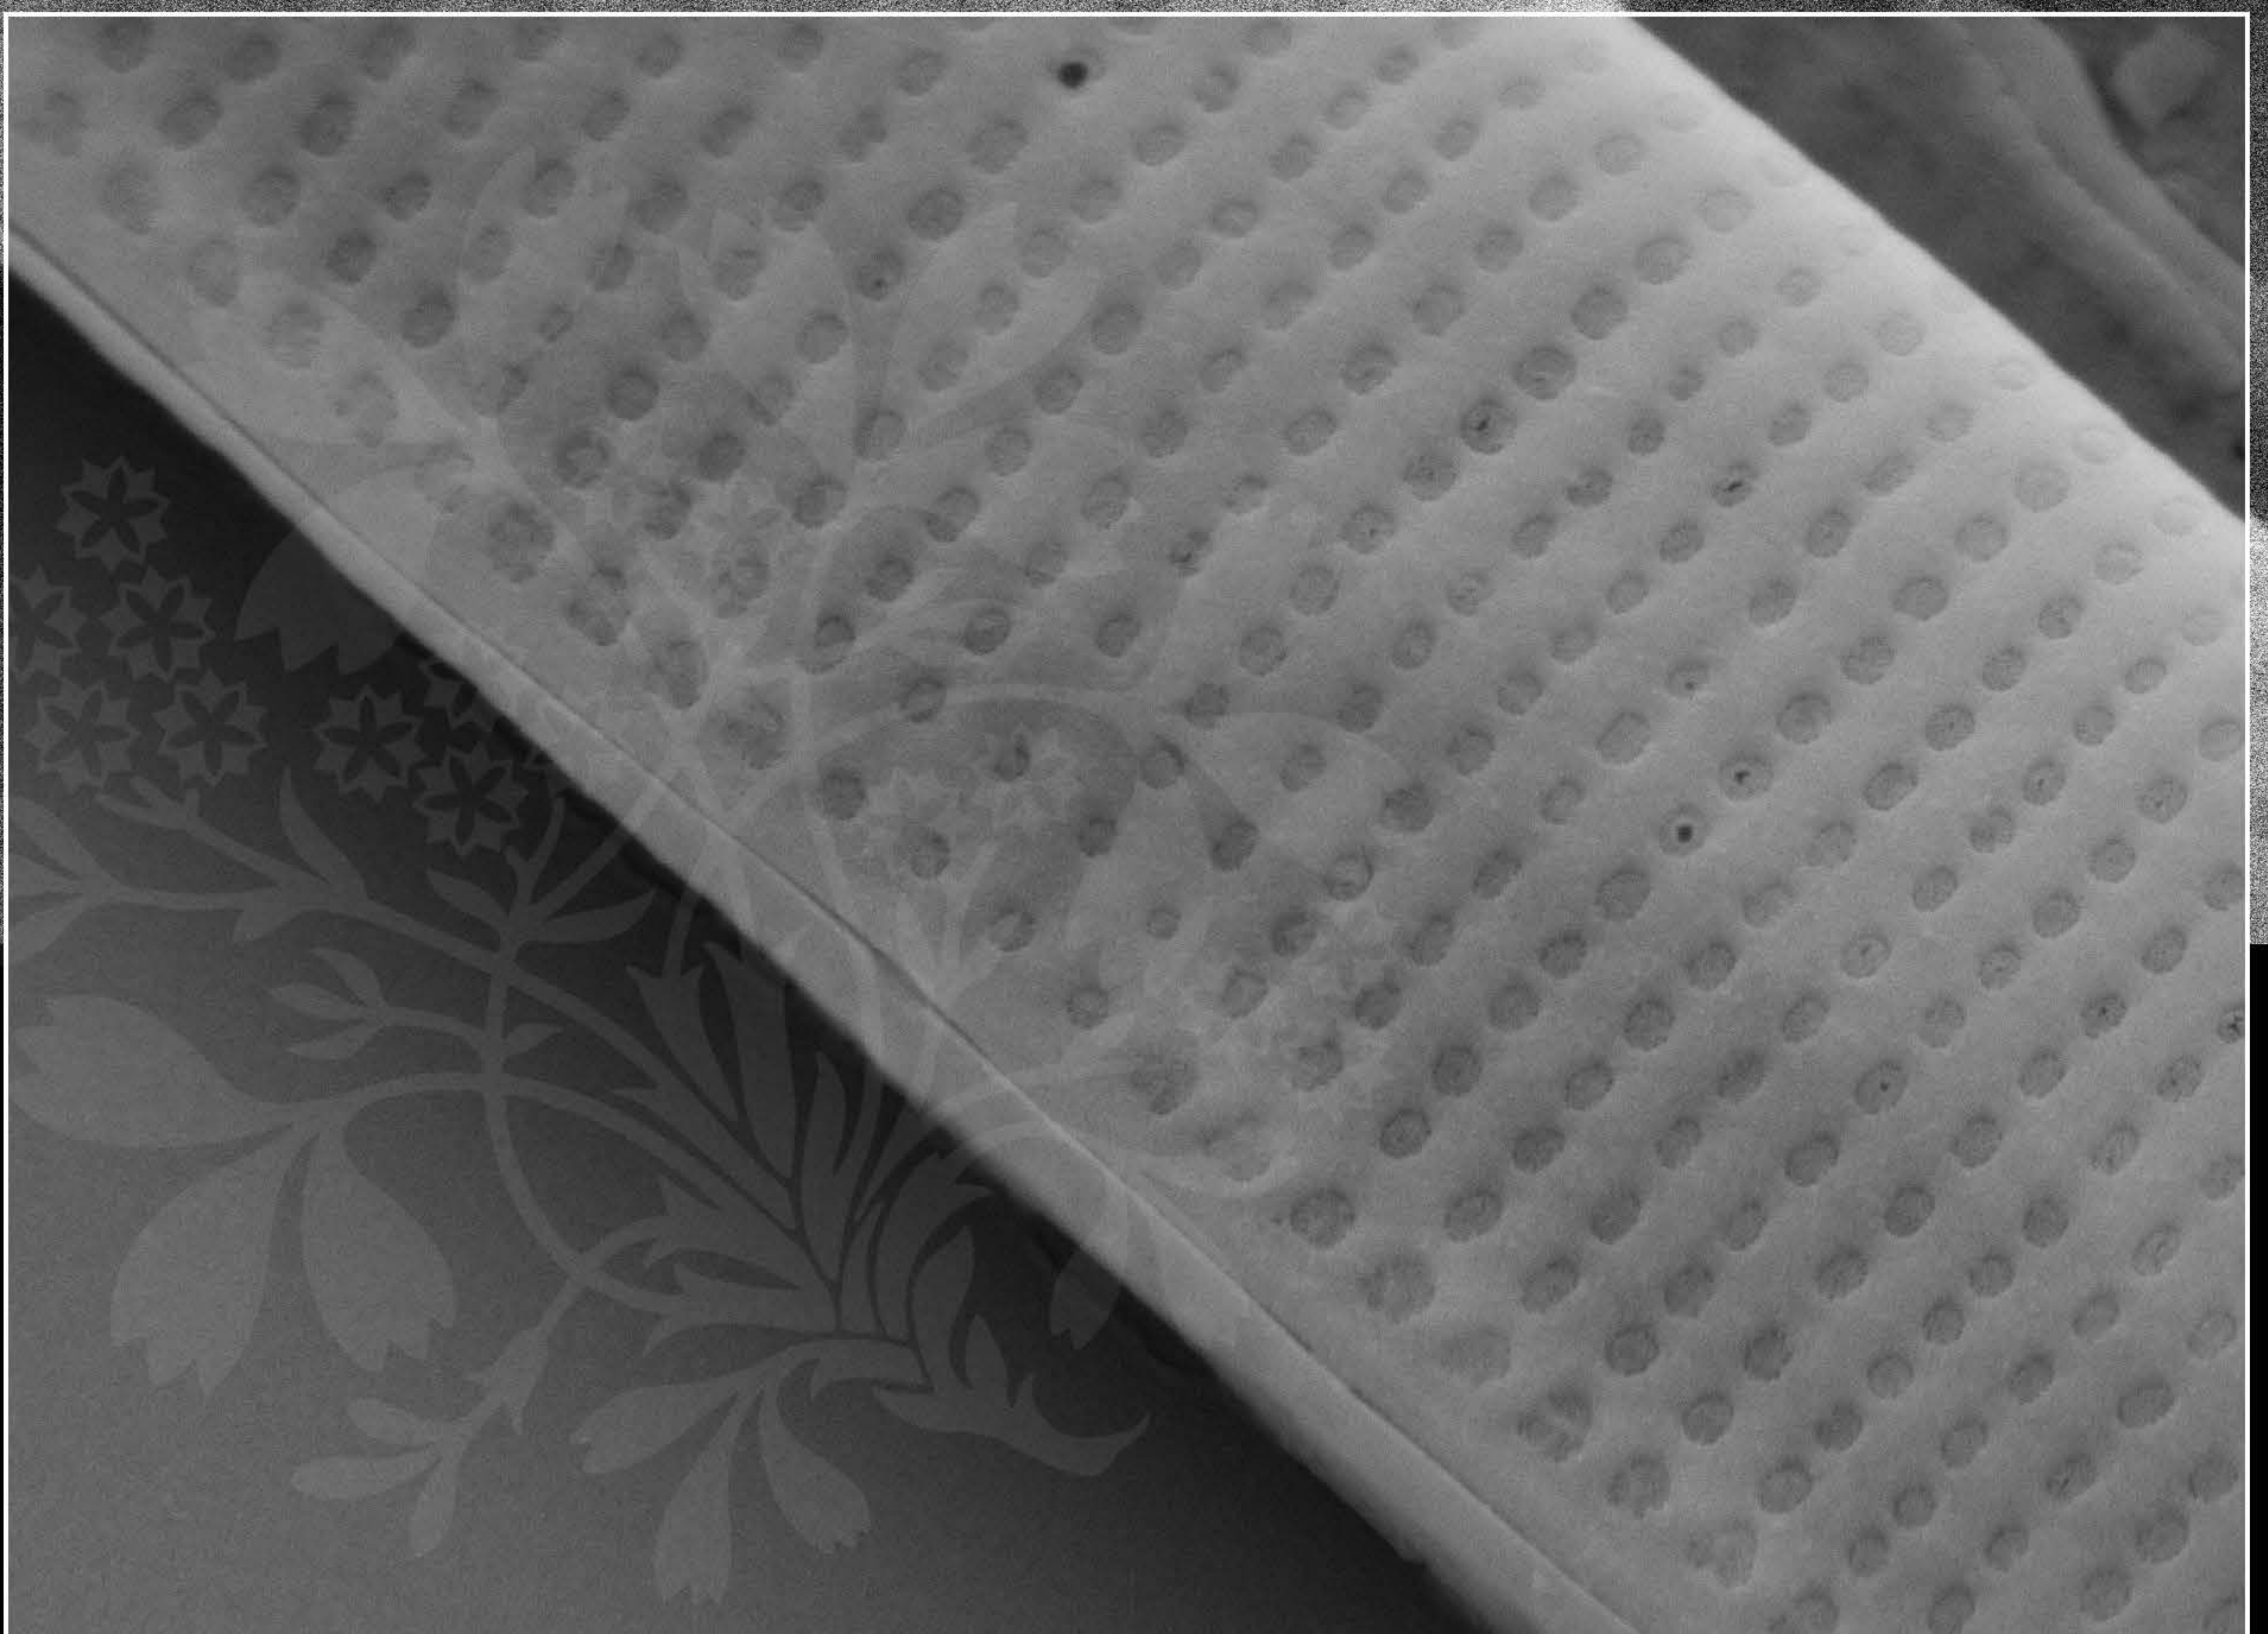

100 nm
└─┘

Mag = 54.26 K X


EHT = 5.00 kV

Signal A = SE2 Date :16 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_10.tif



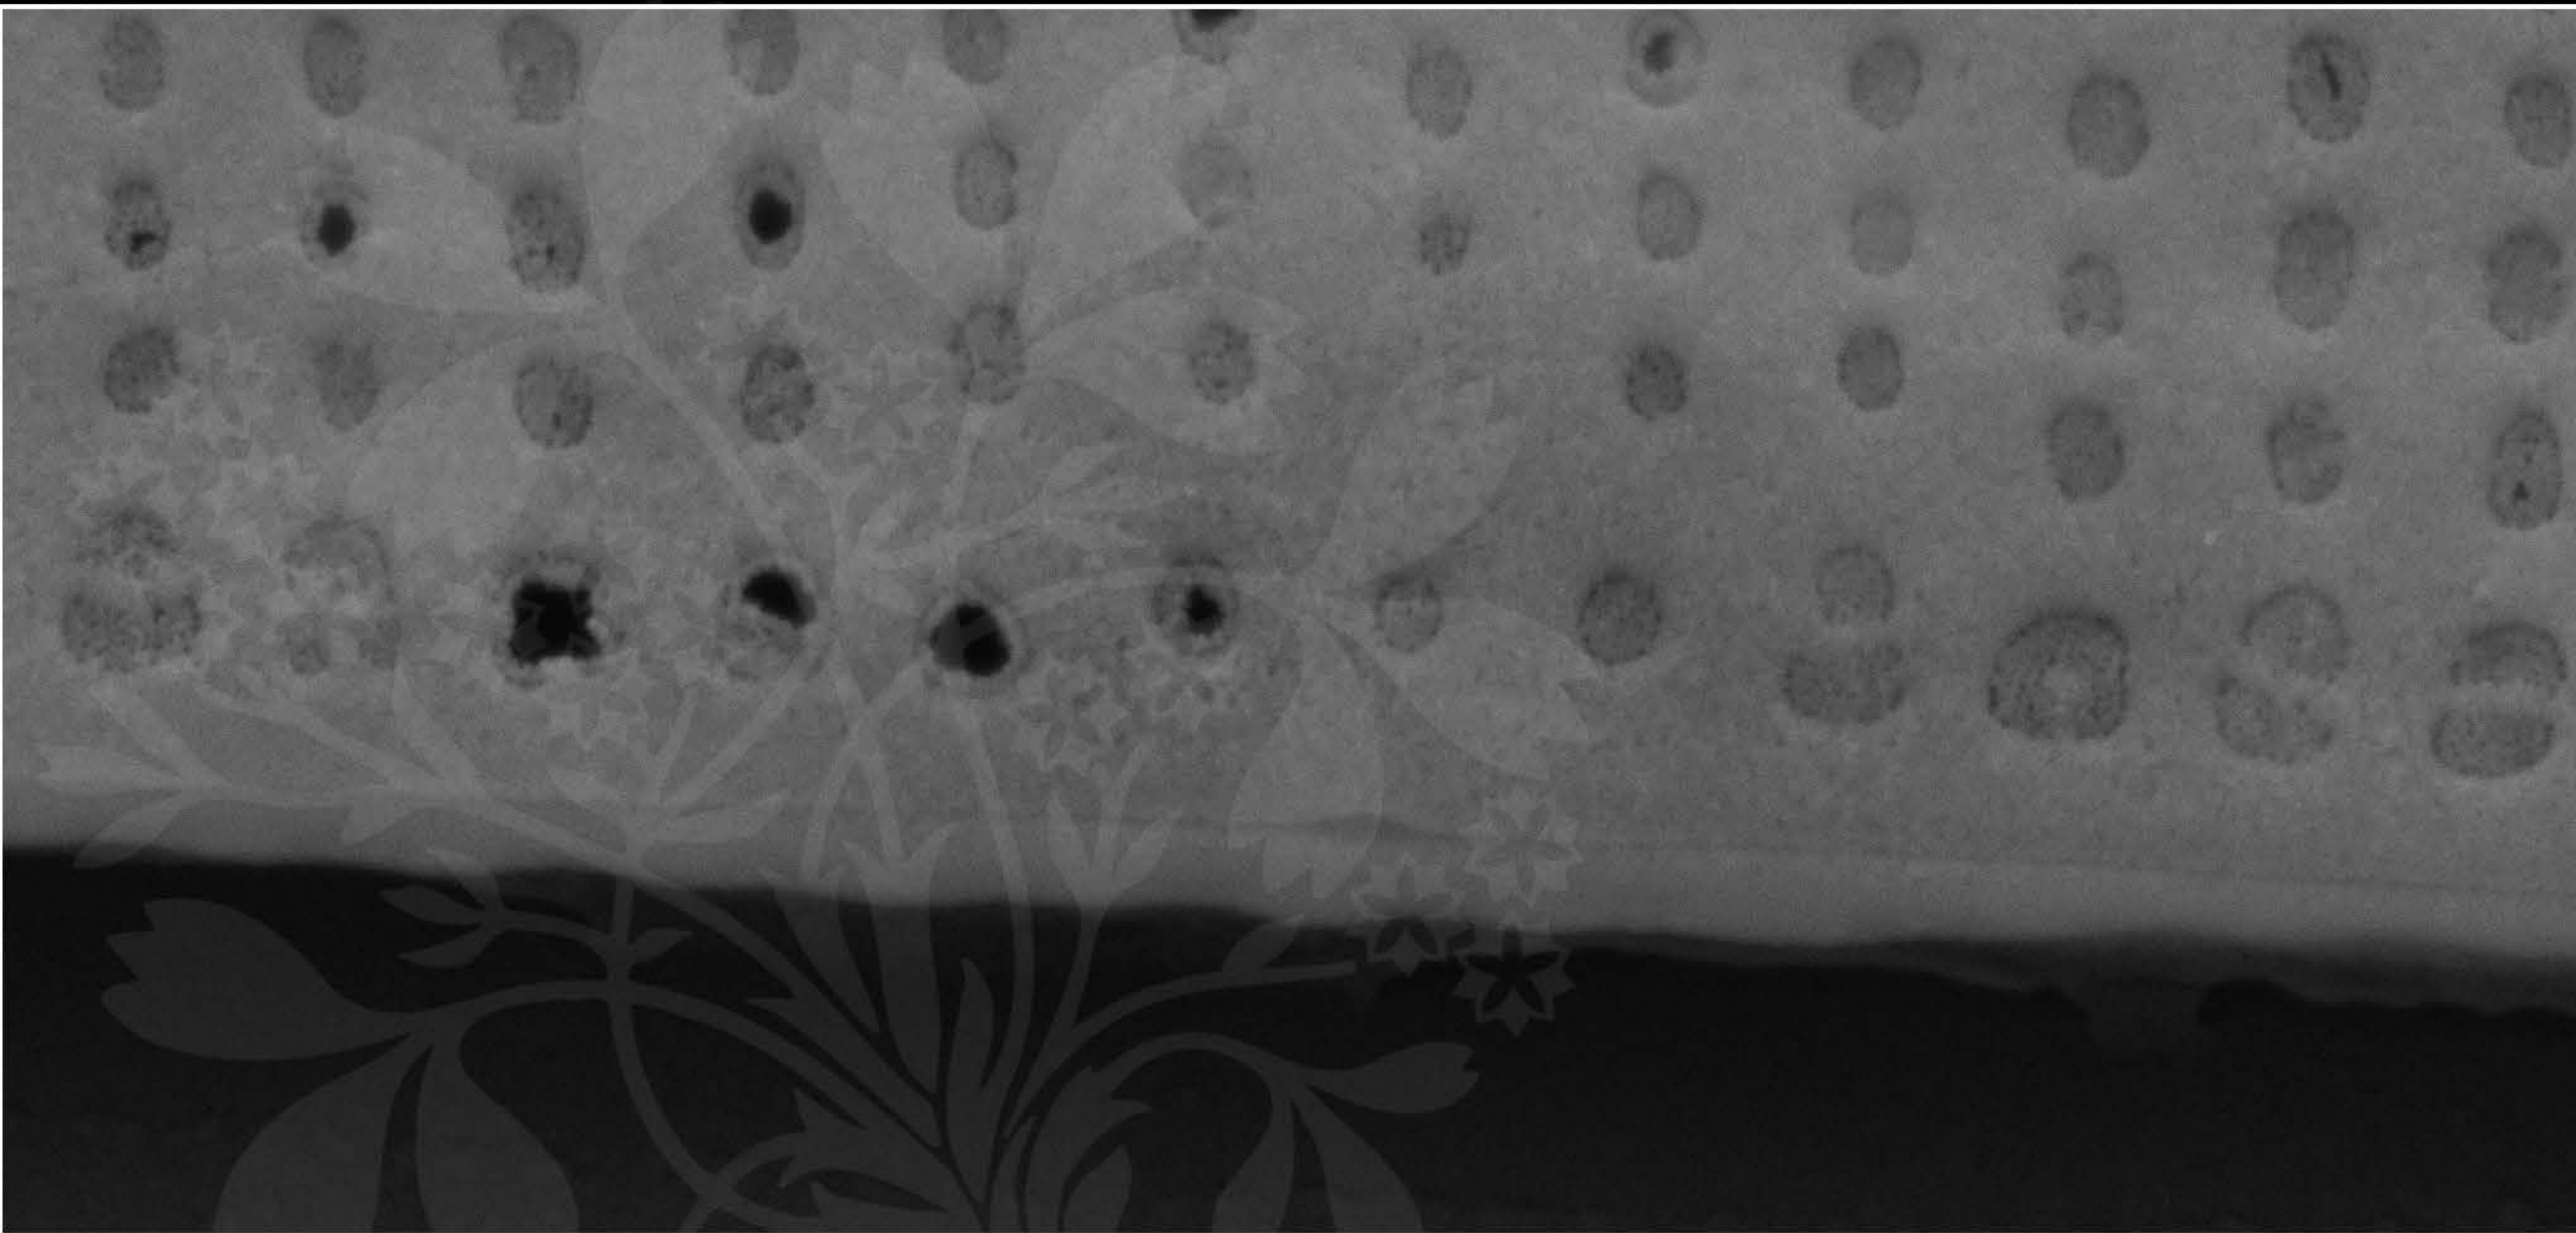

100 nm
└───┘

Mag = 100.00 K X


EHT = 5.00 kV

Signal A = SE2 Date :16 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_11.tif



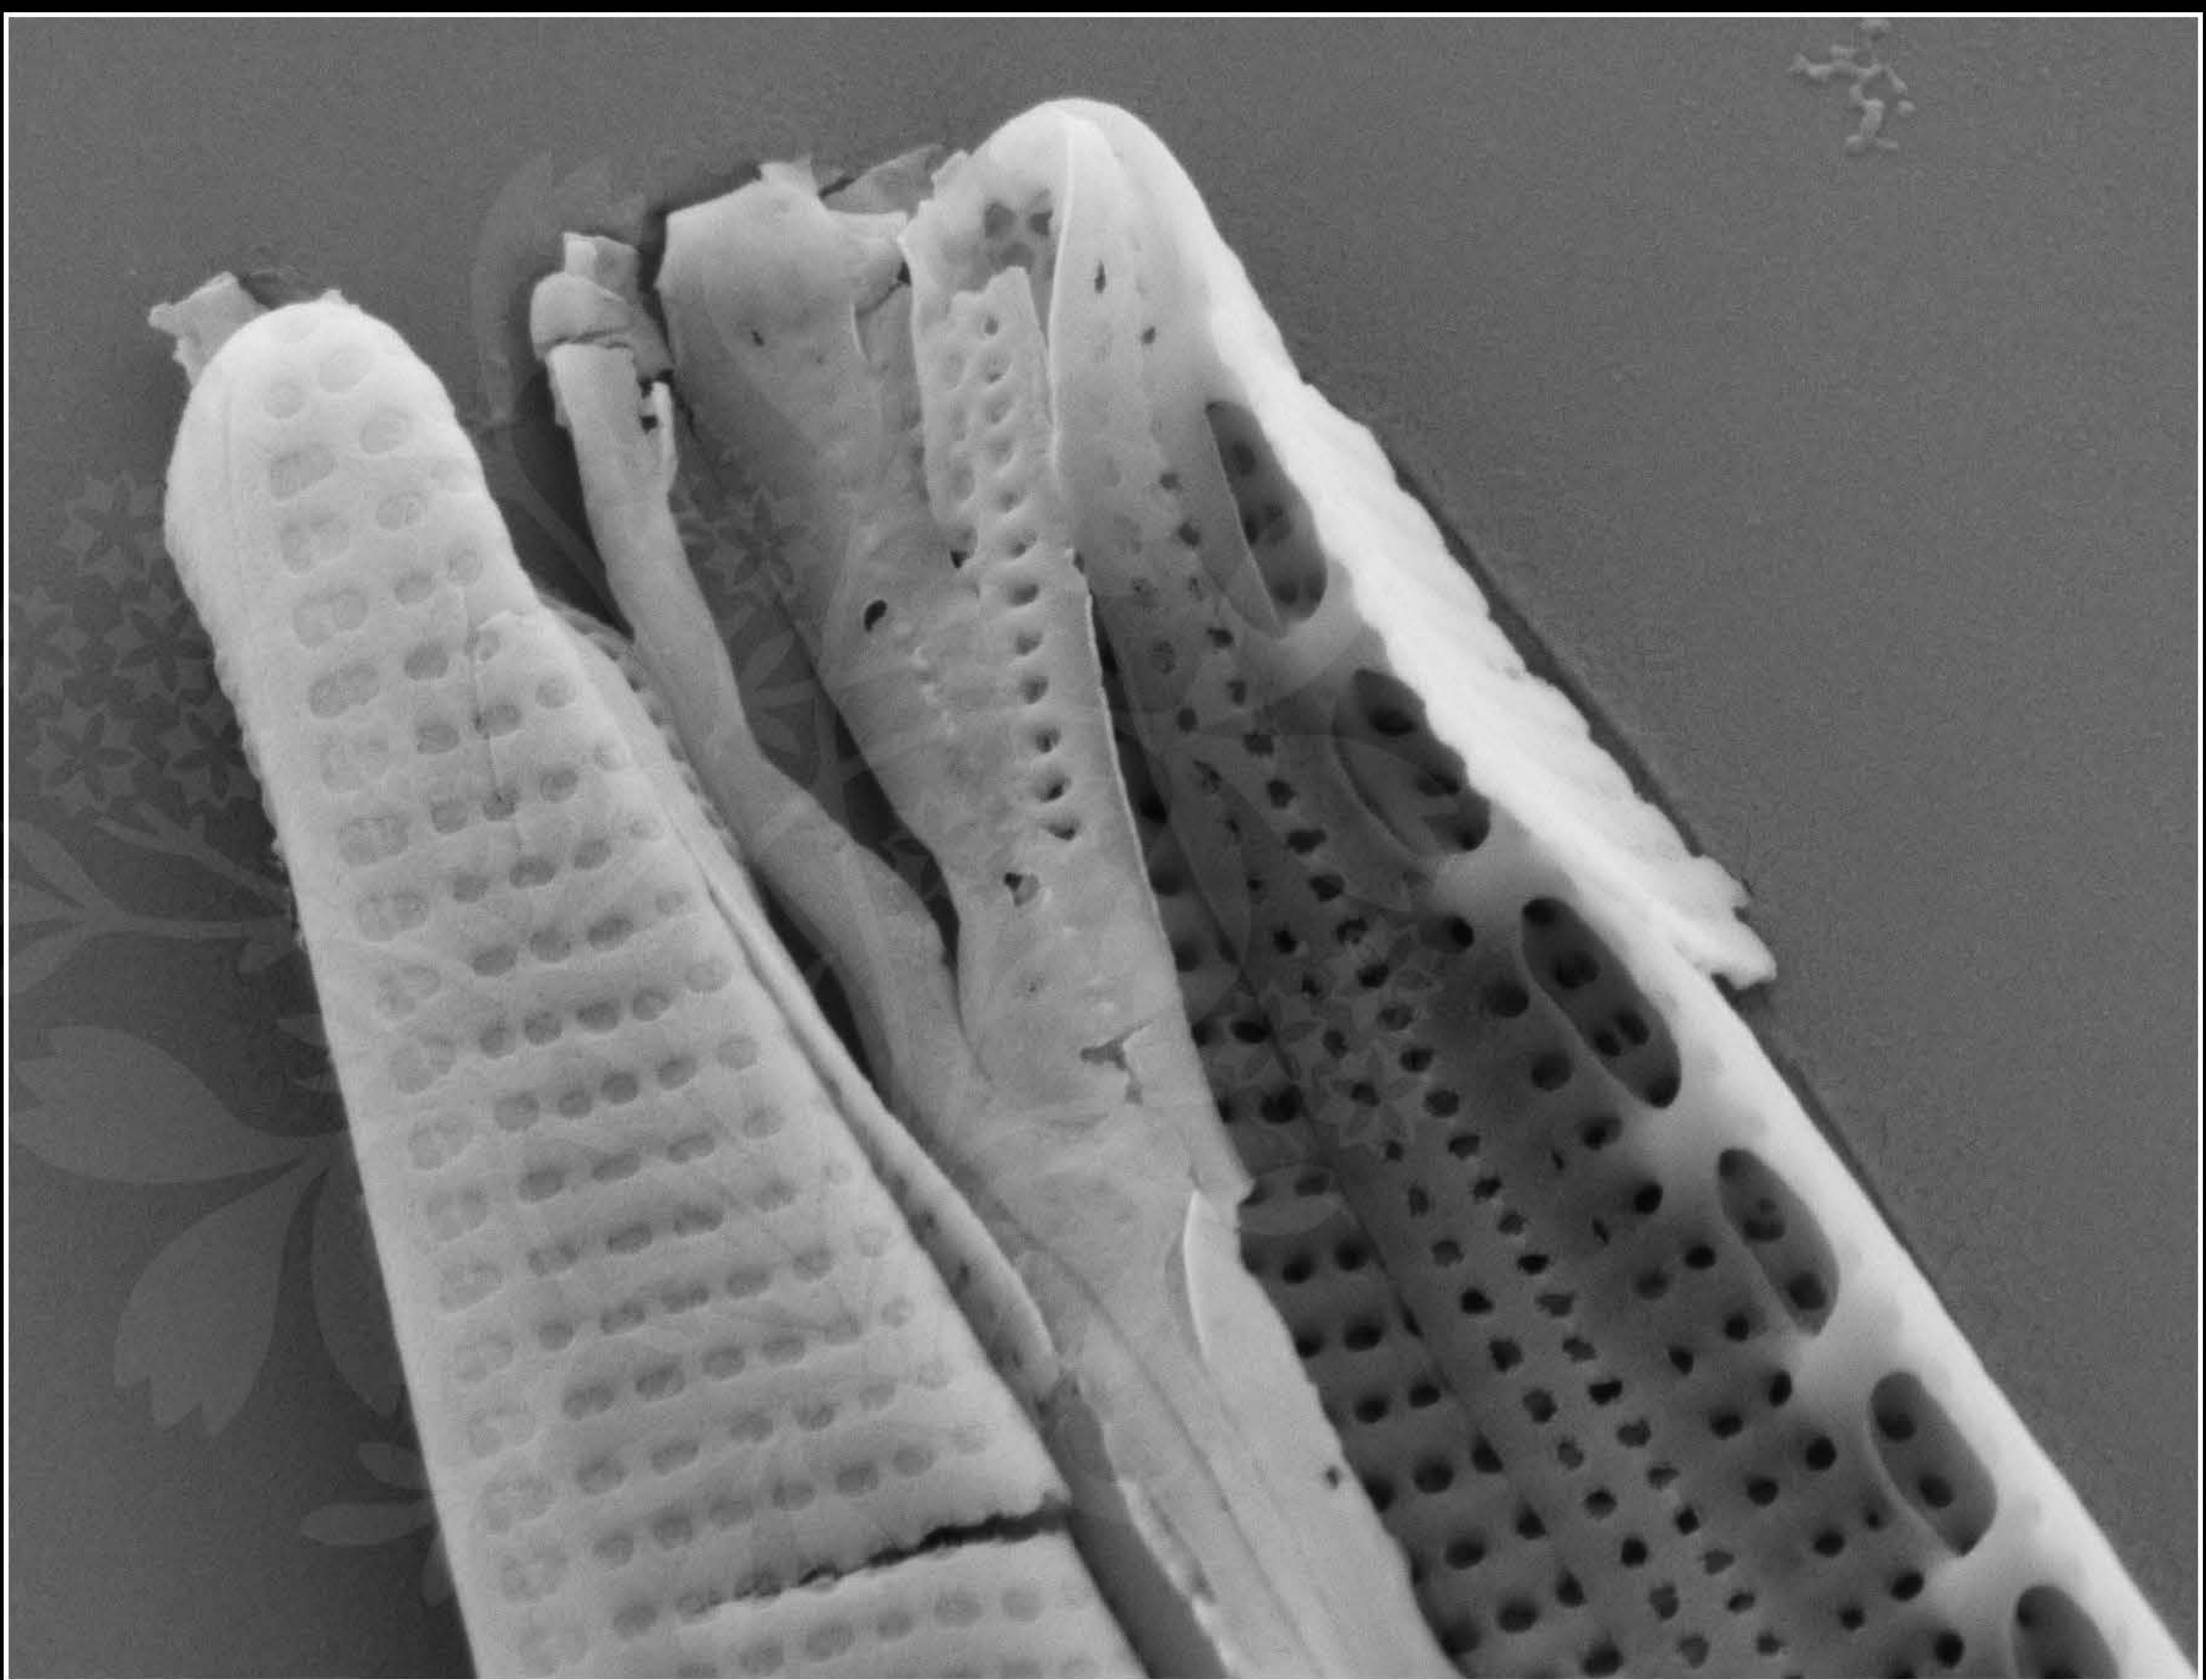

200 nm
└───┘

Mag = 40.00 K X


EHT = 5.00 kV


Signal A = SE2 Date :16 Jun 2017

WD = 4.3 mm

File Name = Barcode0675_12.tif



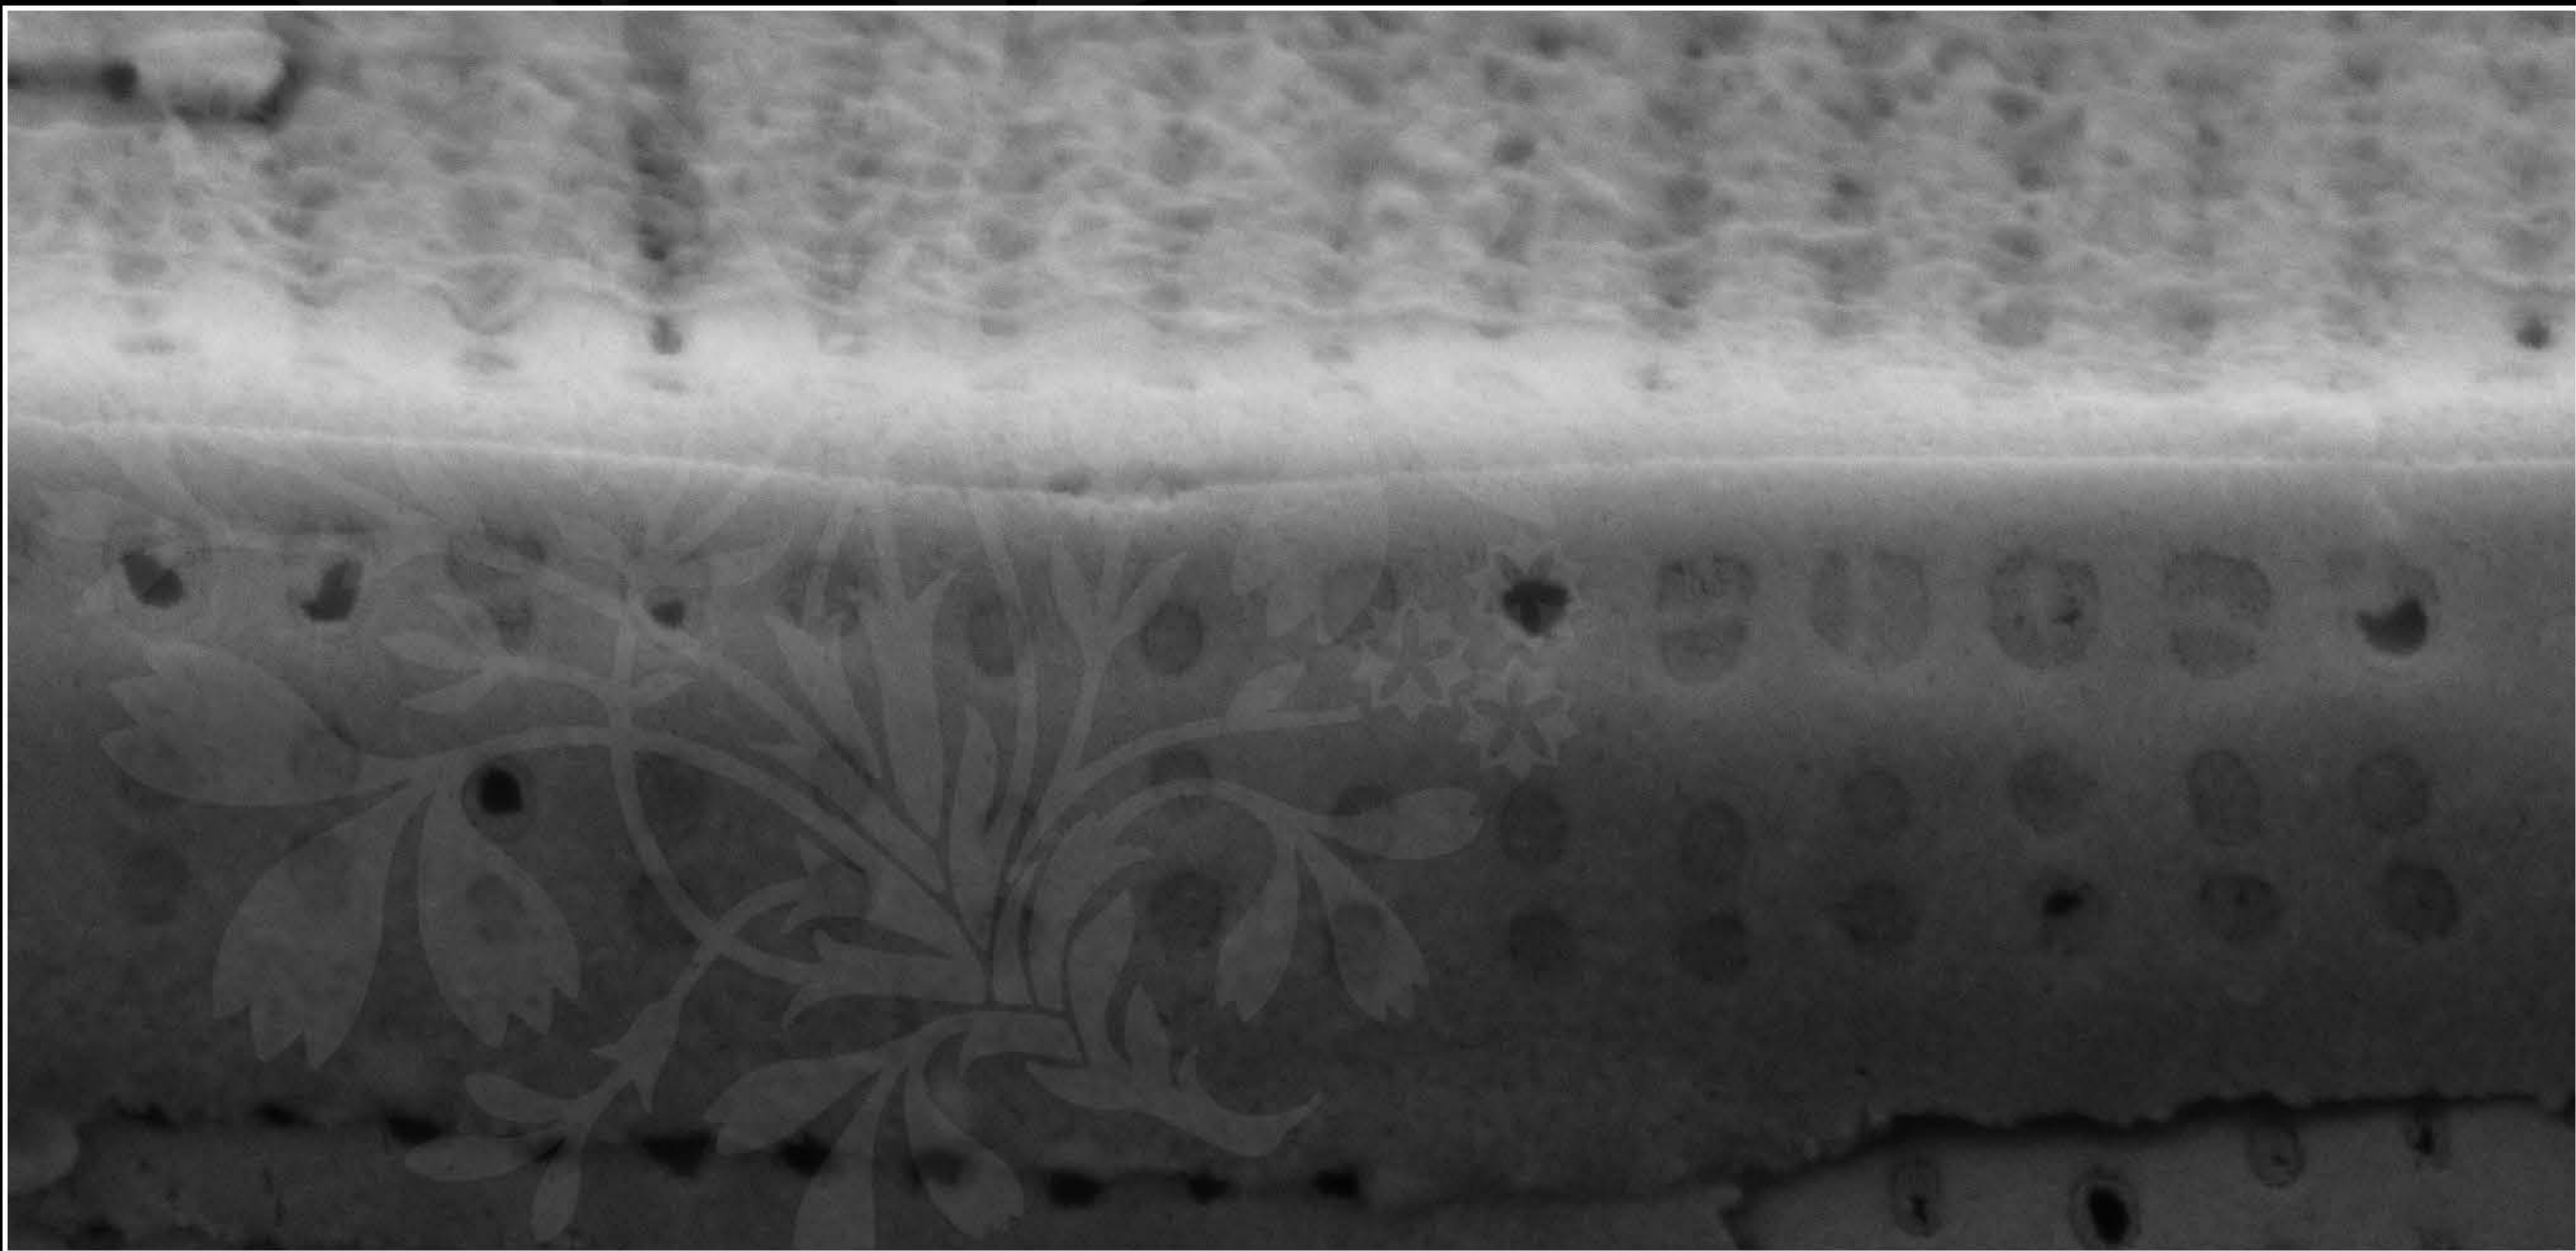

200 nm


Mag = 80.00 K X

EHT = 5.00 kV

Signal A = SE2 Date :16 Jun 2017

WD = 4.2 mm

File Name = Barcode0675_13.tif

